PATENT APPLICATION

25267


PATENT, TRADEMARK OFFICE

THE UNITED STATES PATENT AND TRADEMARK OFFICE

Group: 2632 }
 }
 Atty. Docket: 8266-0519 }
 }
 Applicants: Reeder et al. }
 }
 Invention: PATIENT POINT OF CARE }
 COMPUTER SYSTEM }
 }
 Serial No.: 09/849,580 }
 }
 Filed: May 4, 2001 }
 }
 Examiner: Unknown }

Certificate Under 37 CFR 1.8(a)

I hereby certify that this correspondence is being
 deposited with the United States Postal Service
 with sufficient postage for first class mail in an
 envelope addressed to Box Issue Fee, Assistant
 Commissioner for Patents, Washington, D.C.
 20231

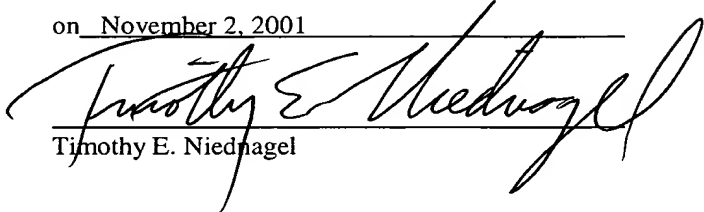on November 2, 2001

 Timothy E. Niednagel
LETTER TO OFFICIAL DRAFTSMAN

Box Missing Parts
 Commissioner for Patents
 Washington, D.C. 20231


Dear Sir:

Applicants submit herewith formal drawings for the above-identified application
 meeting the requirements of 37 CFR Section 1.84.

If the Draftsman has any questions regarding the drawings, please contact applicants'
 undersigned attorney, at (317) 684-5251.

Respectfully submitted,

BOSE McKINNEY & EVANS LLP

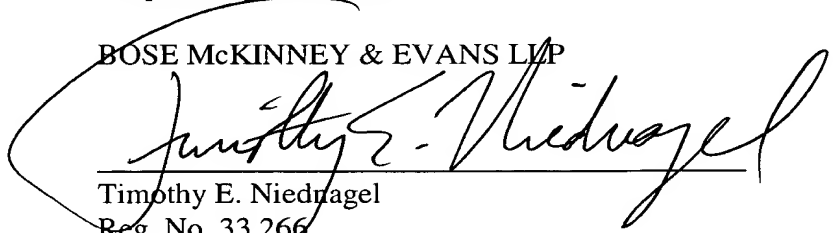
 Timothy E. Niednagel
 Reg. No. 33,266

TEN:kyb
 Indianapolis, Indiana
 (317) 684-5251
 ::ODMA\MHODMA\DT1;268510;1

09849580-121801

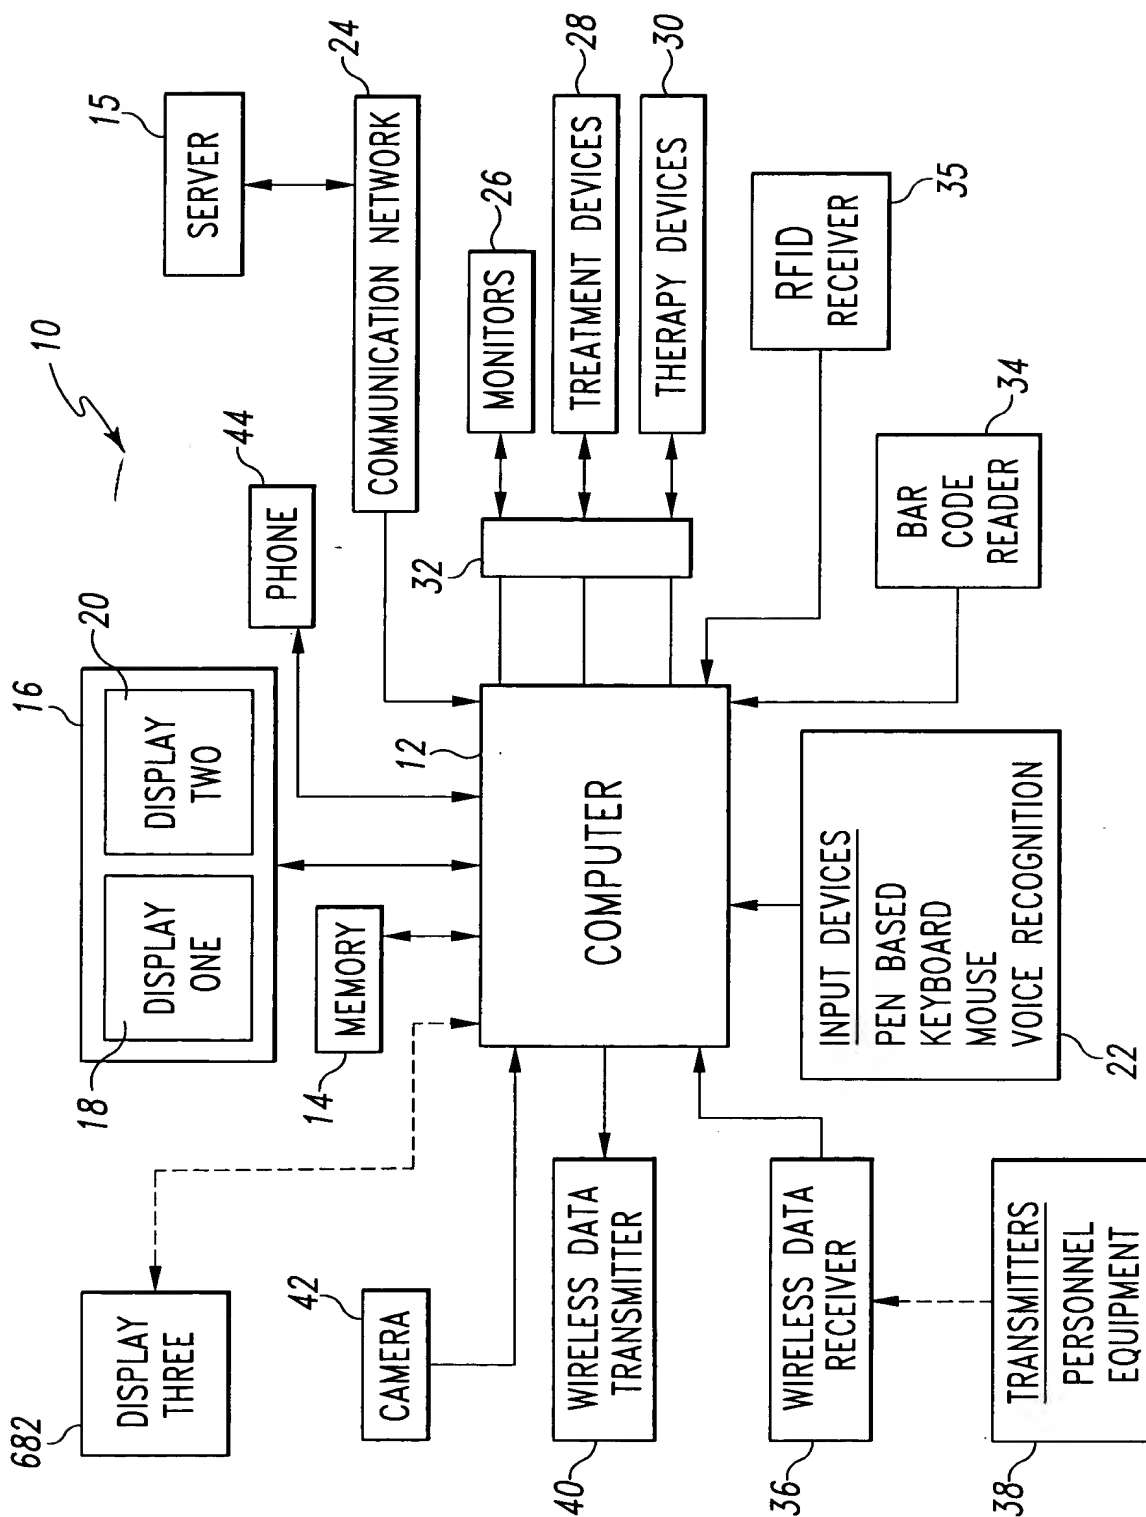


Fig. 1

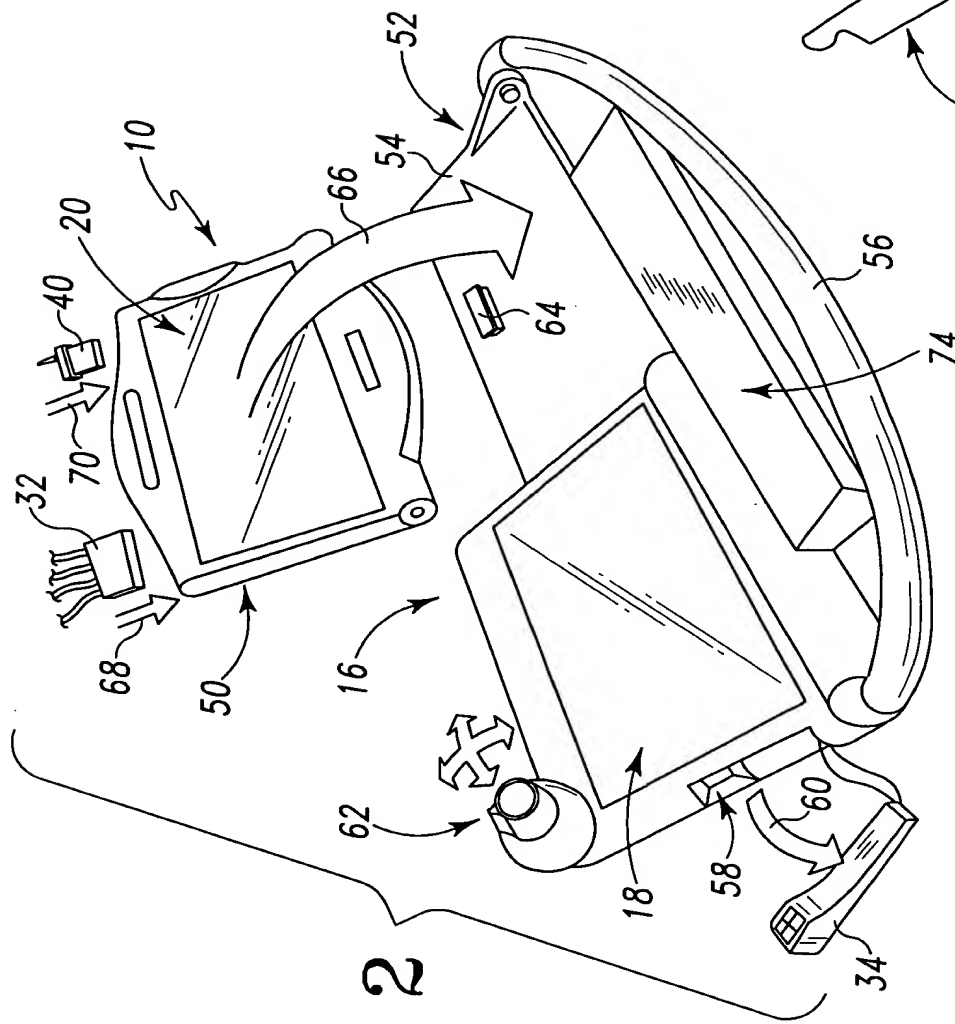


Fig. 2

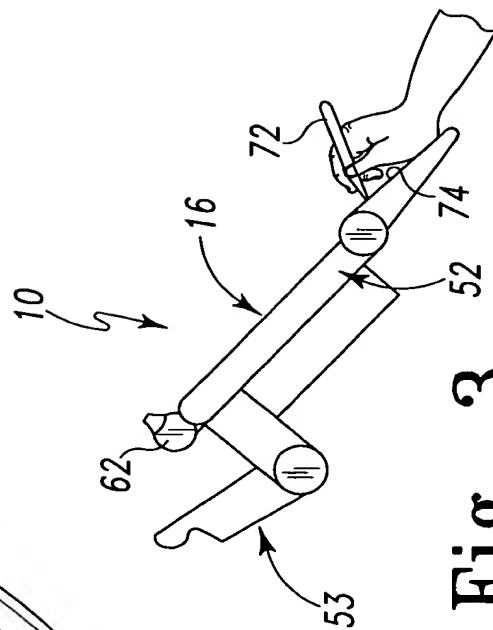


Fig. 3

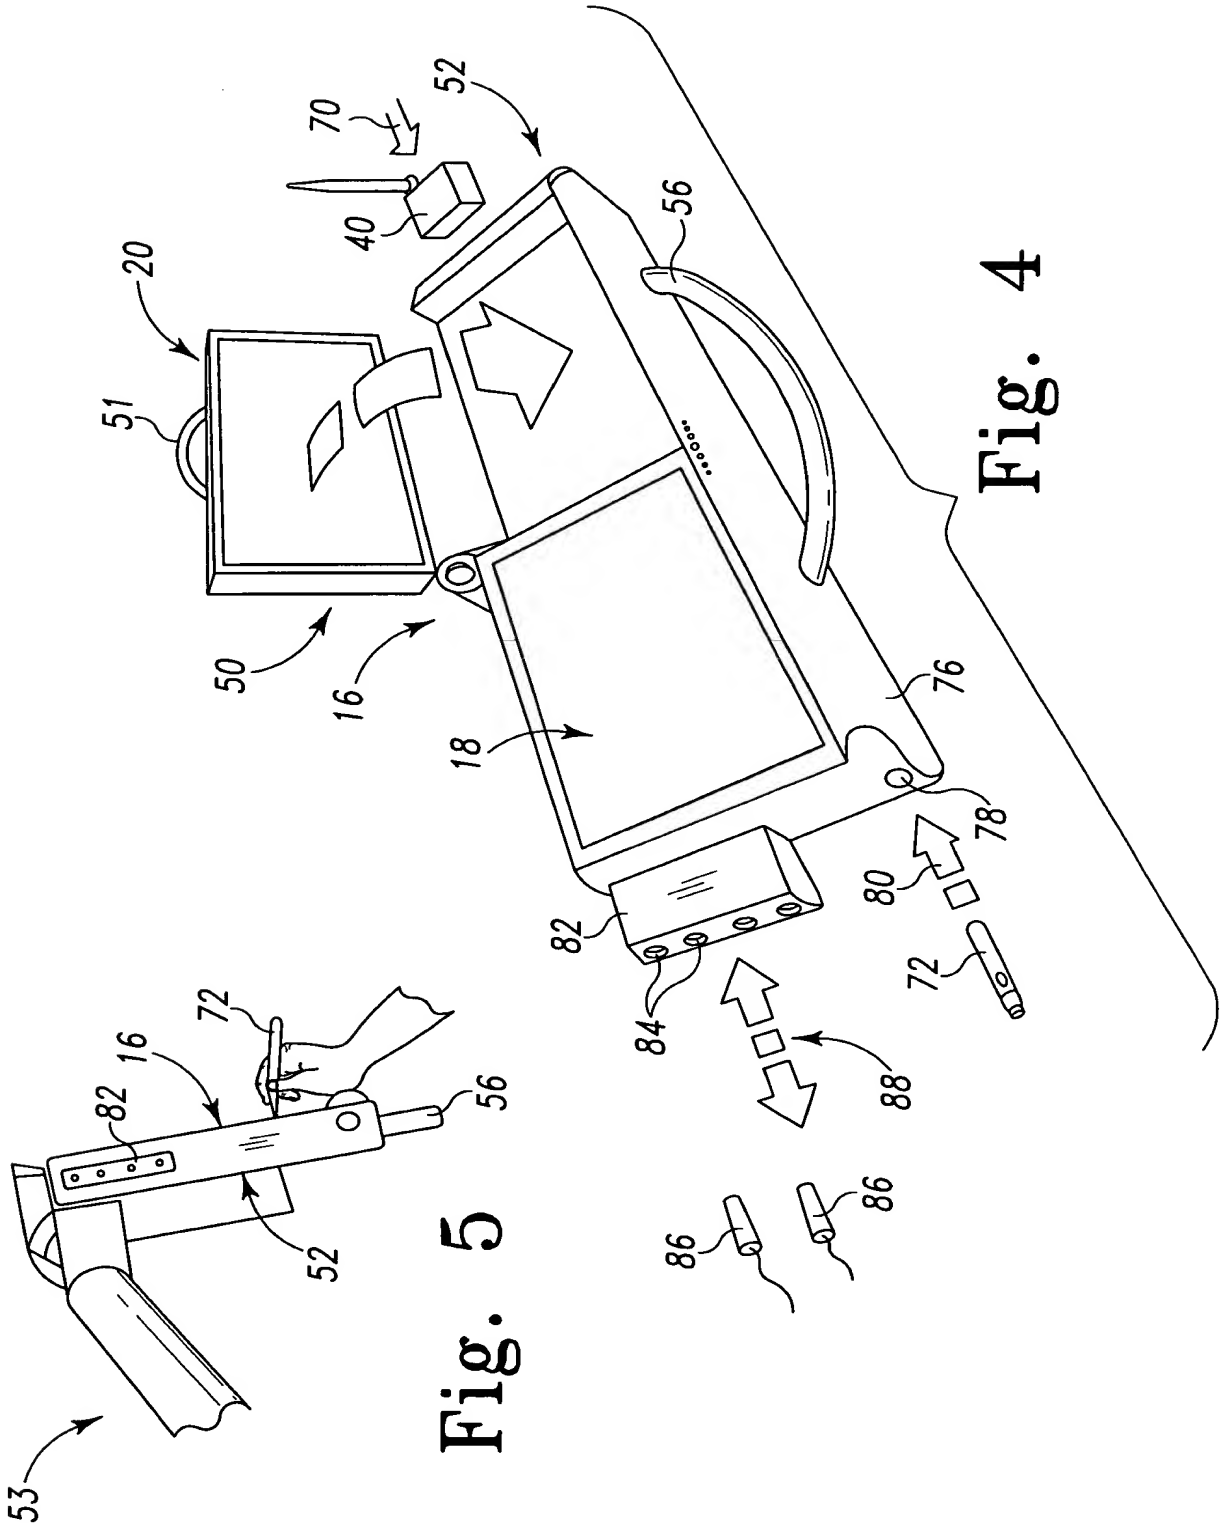


Fig. 4

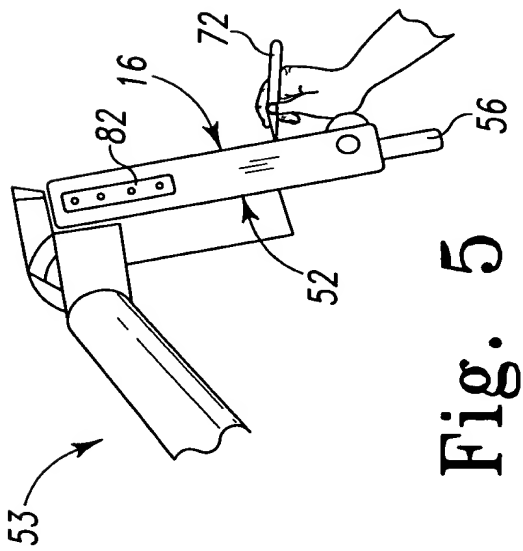


Fig. 5

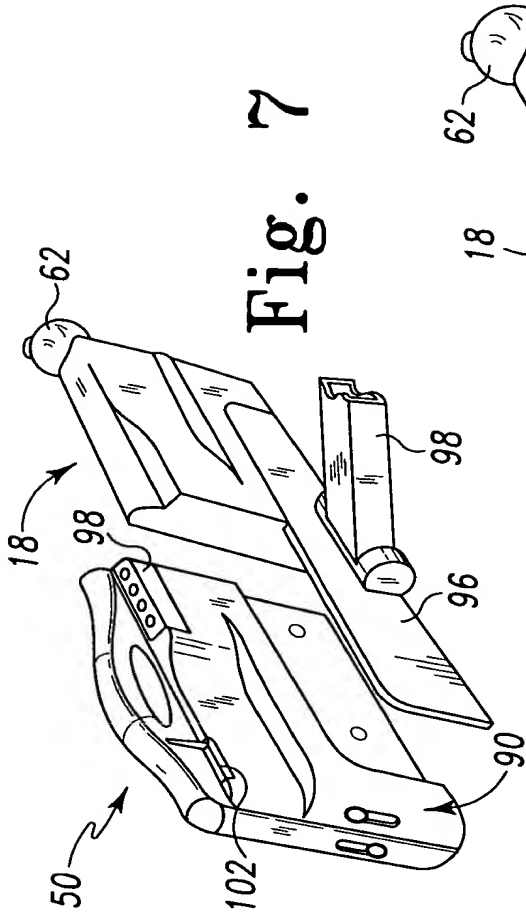


Fig. 7

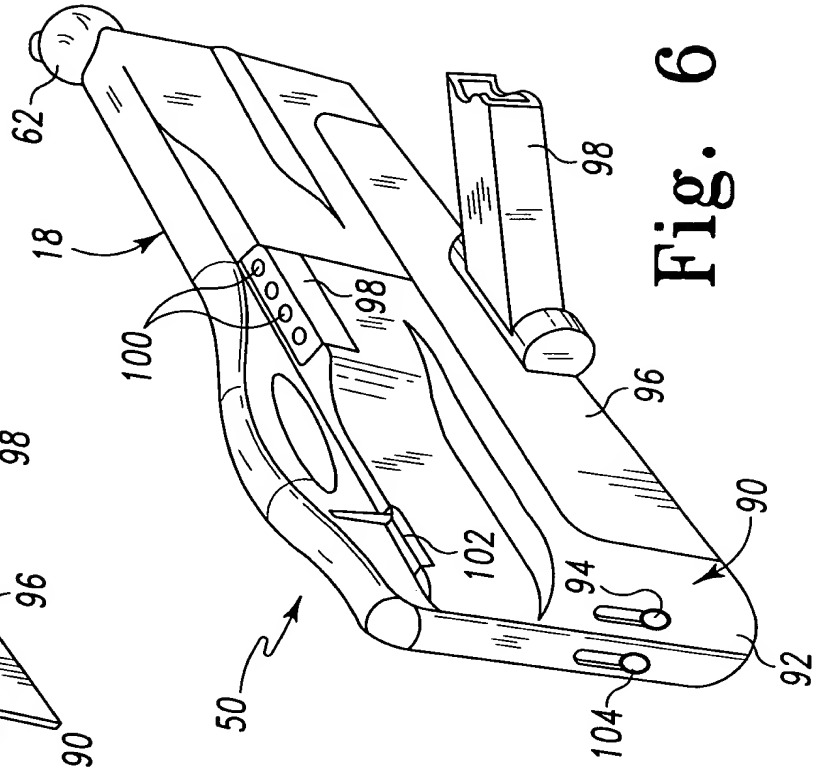


Fig. 6

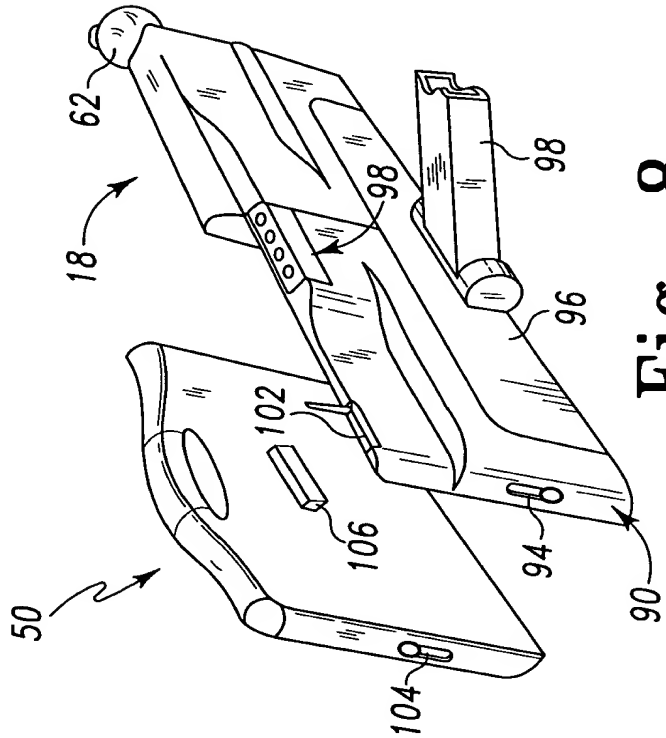


Fig. 8

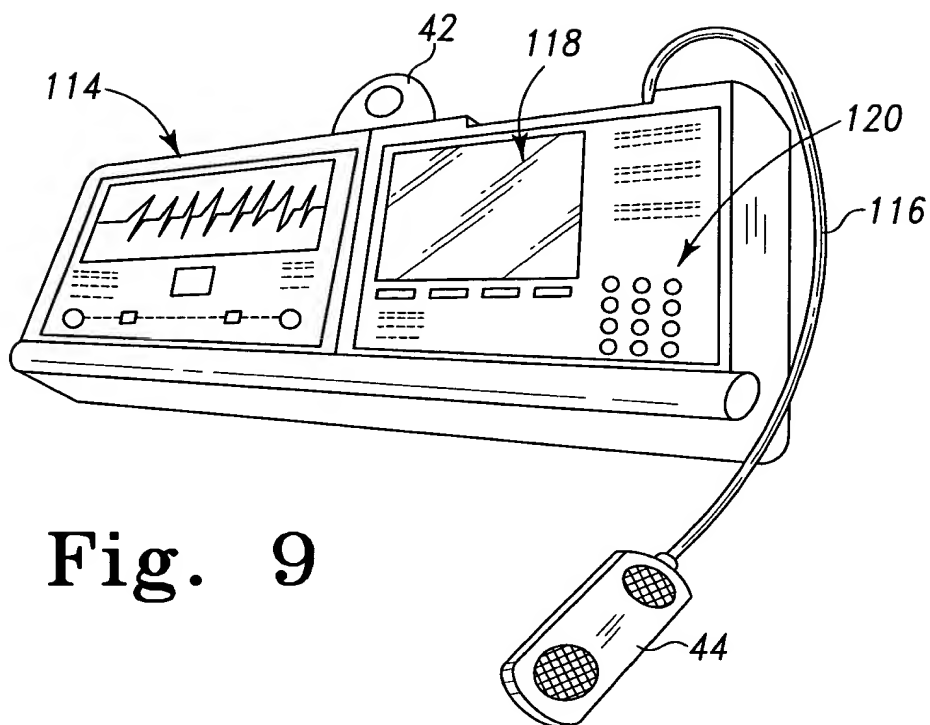


Fig. 9

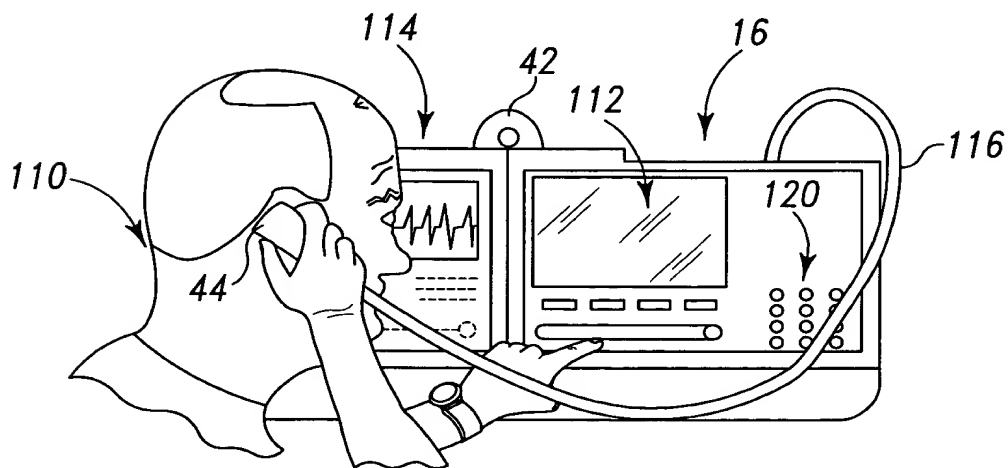


Fig. 10

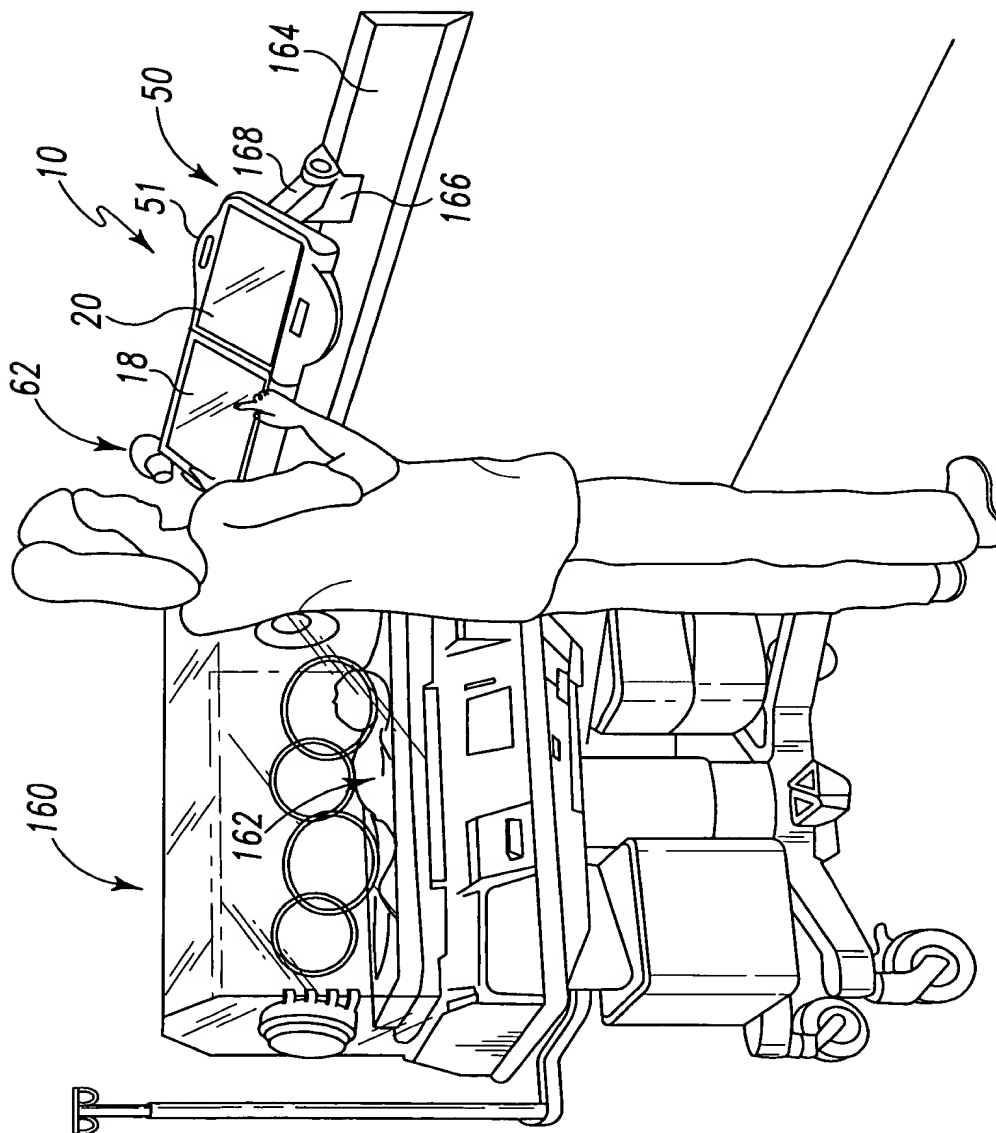


Fig. 12

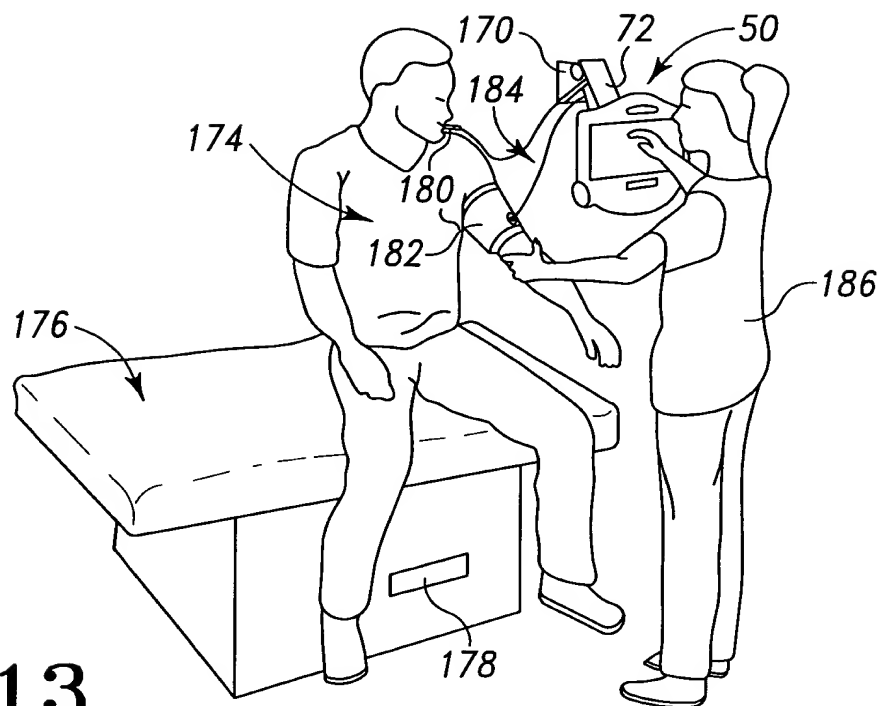


Fig. 13

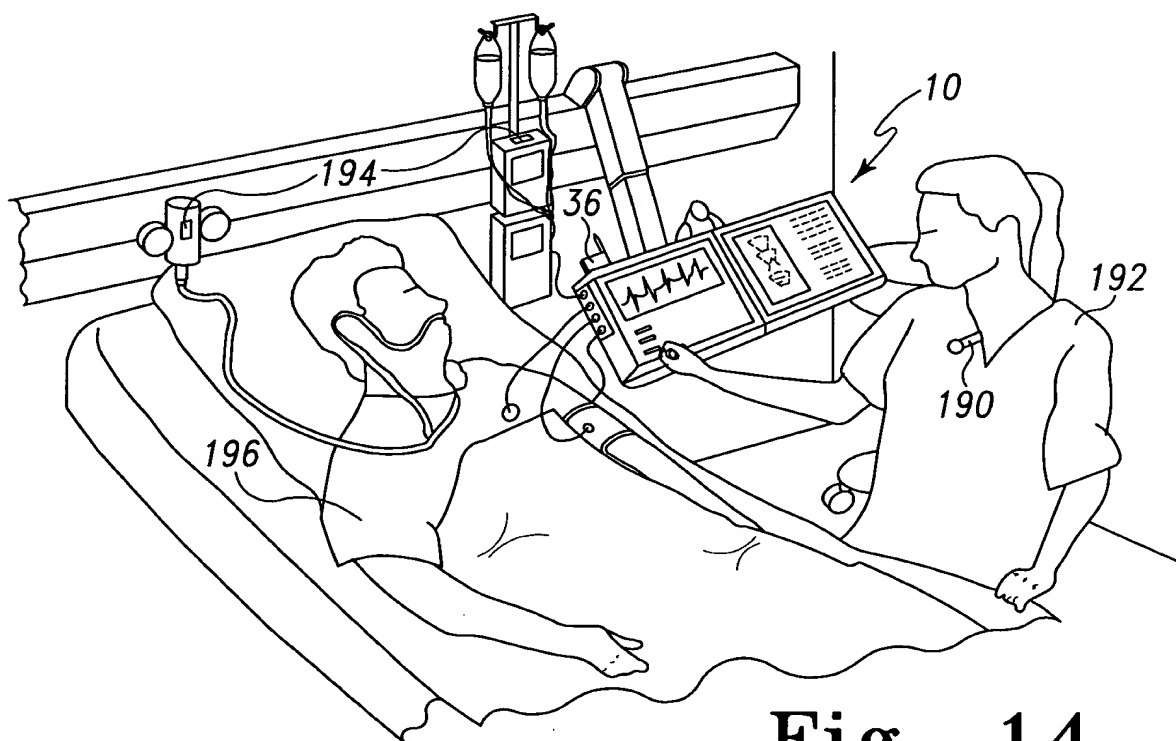


Fig. 14

9/59

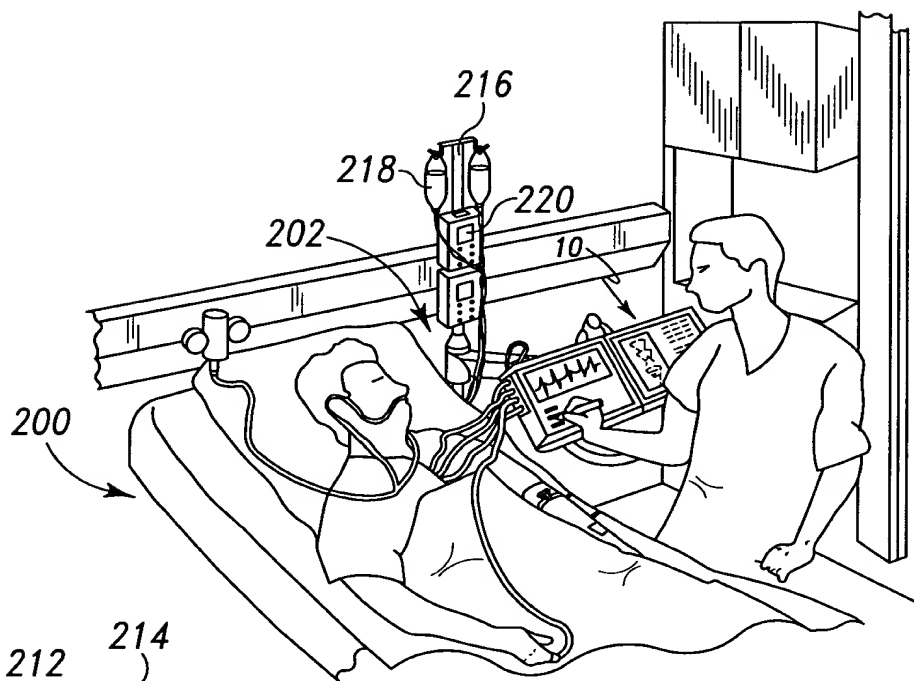


Fig. 15

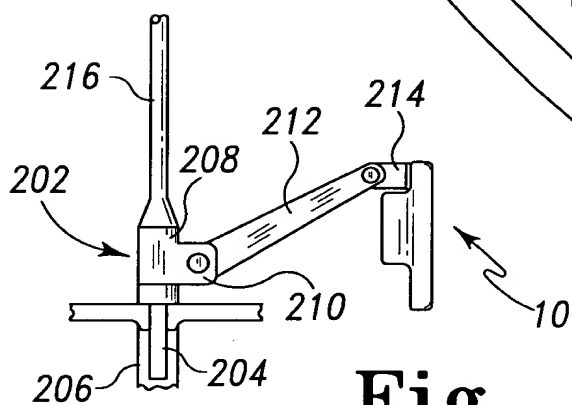


Fig. 16

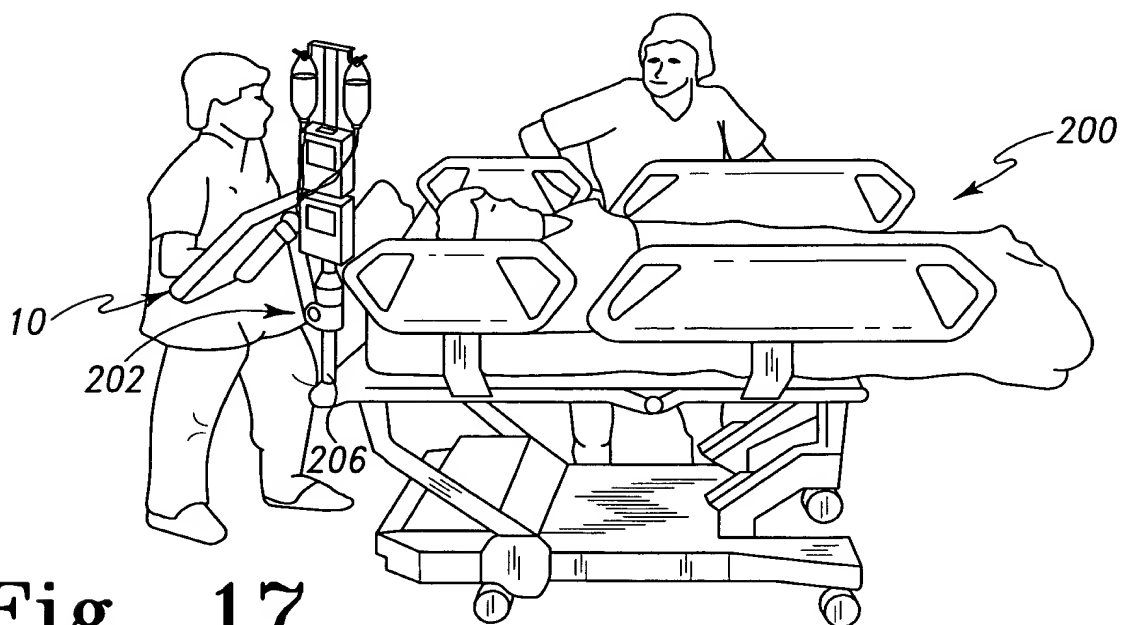


Fig. 17

09549580-121801

10/59

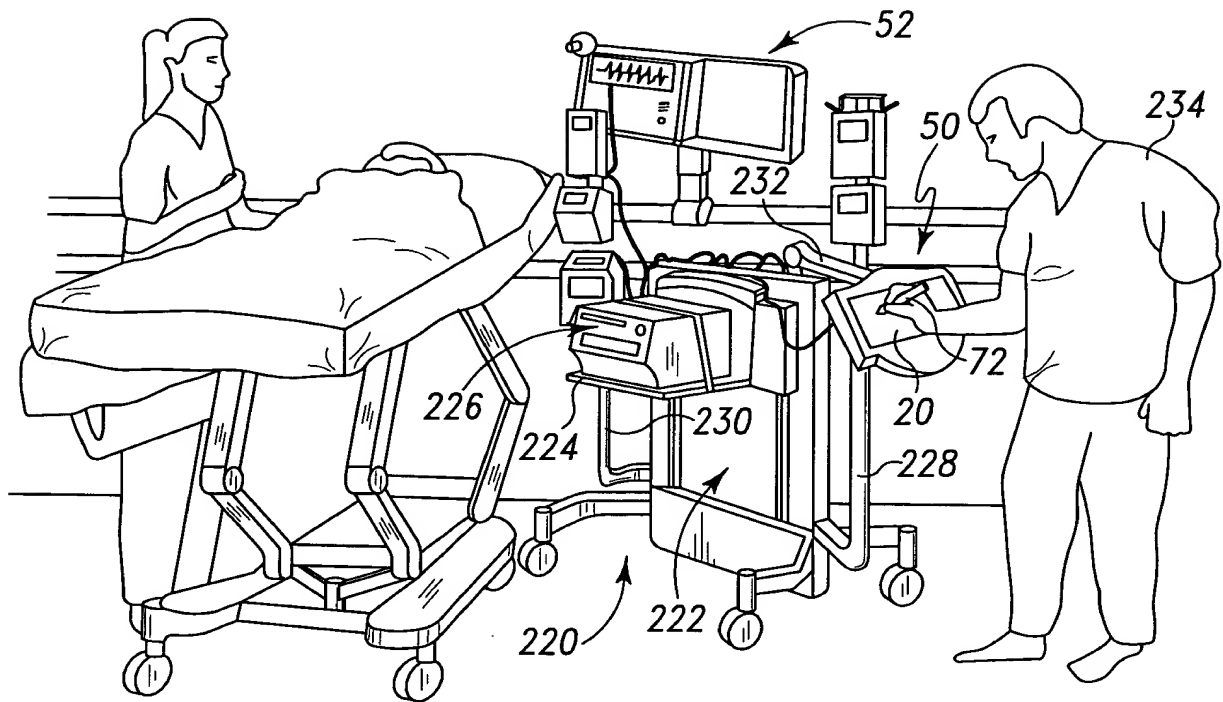


Fig. 18

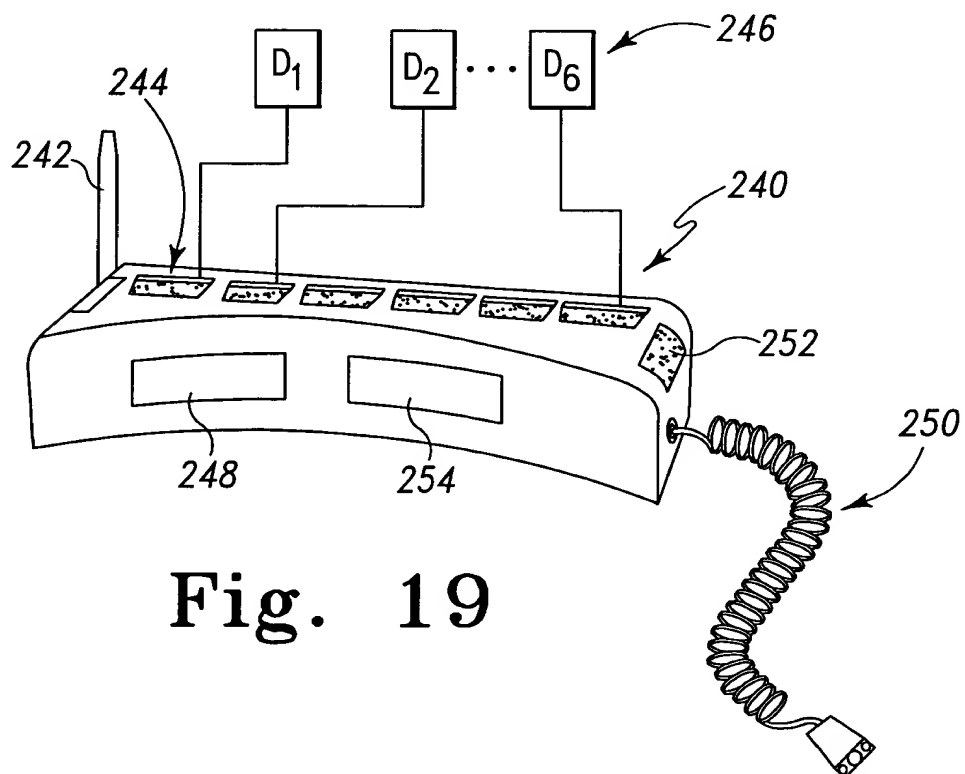


Fig. 19

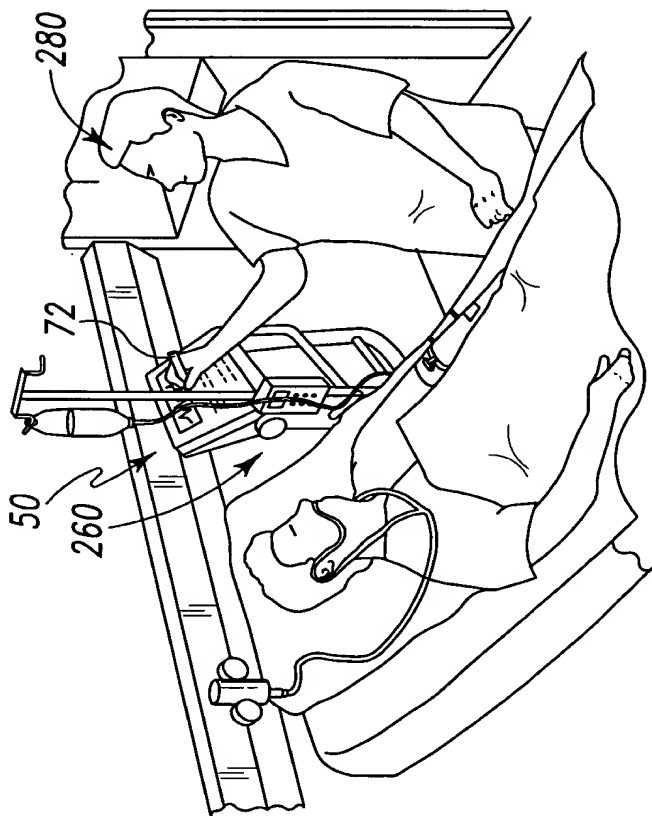


Fig. 21

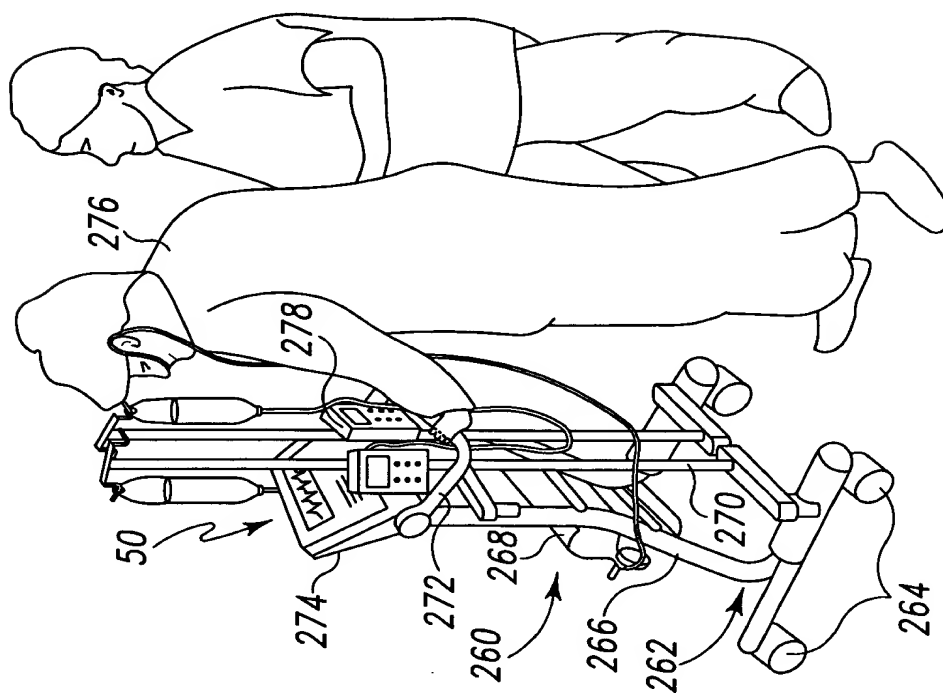


Fig. 20

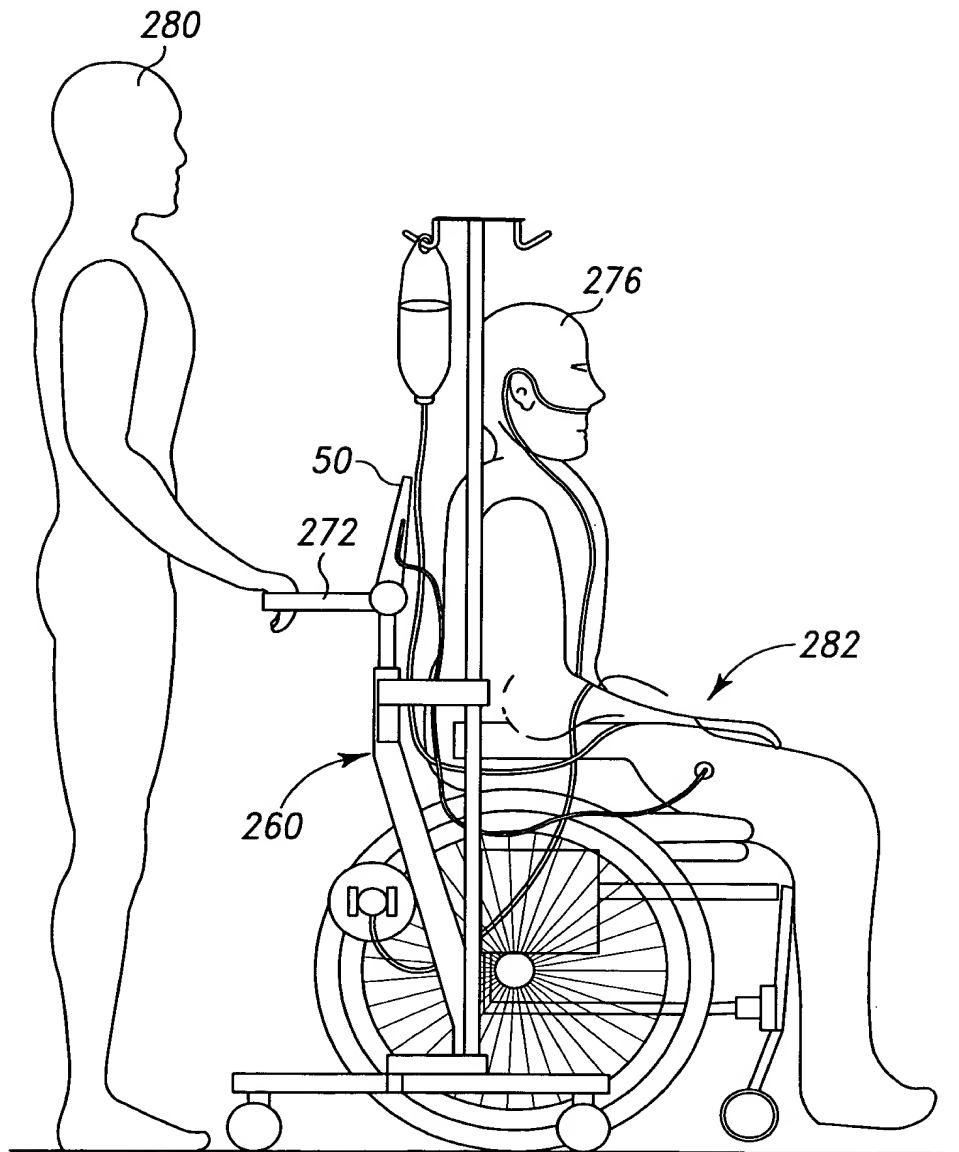


Fig. 22

09849580-121801

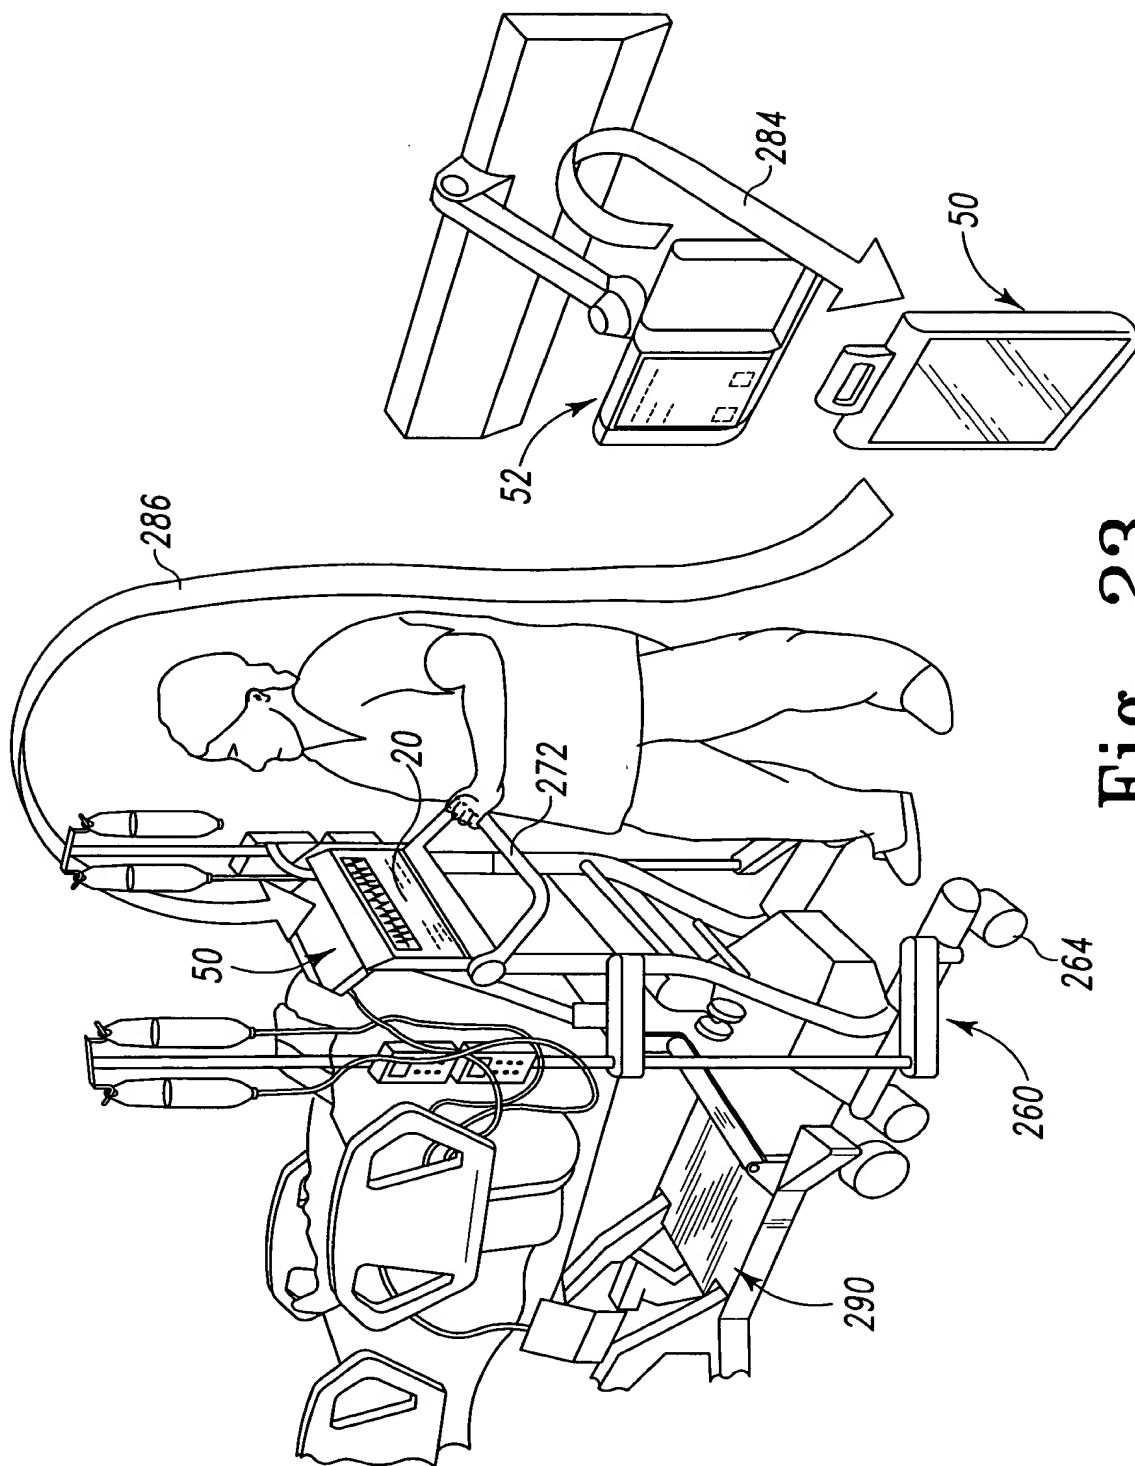


Fig. 23

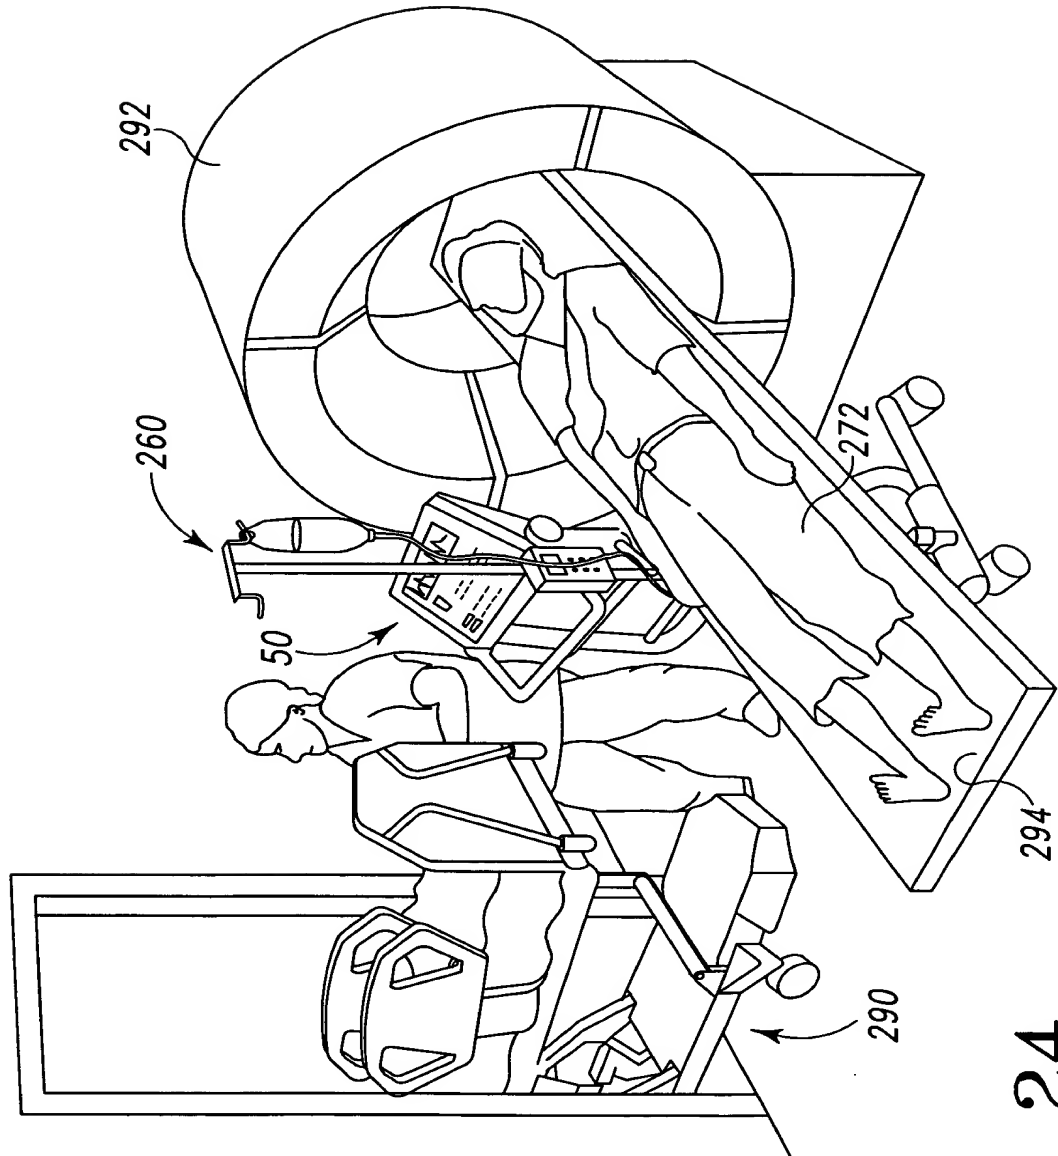


Fig. 24

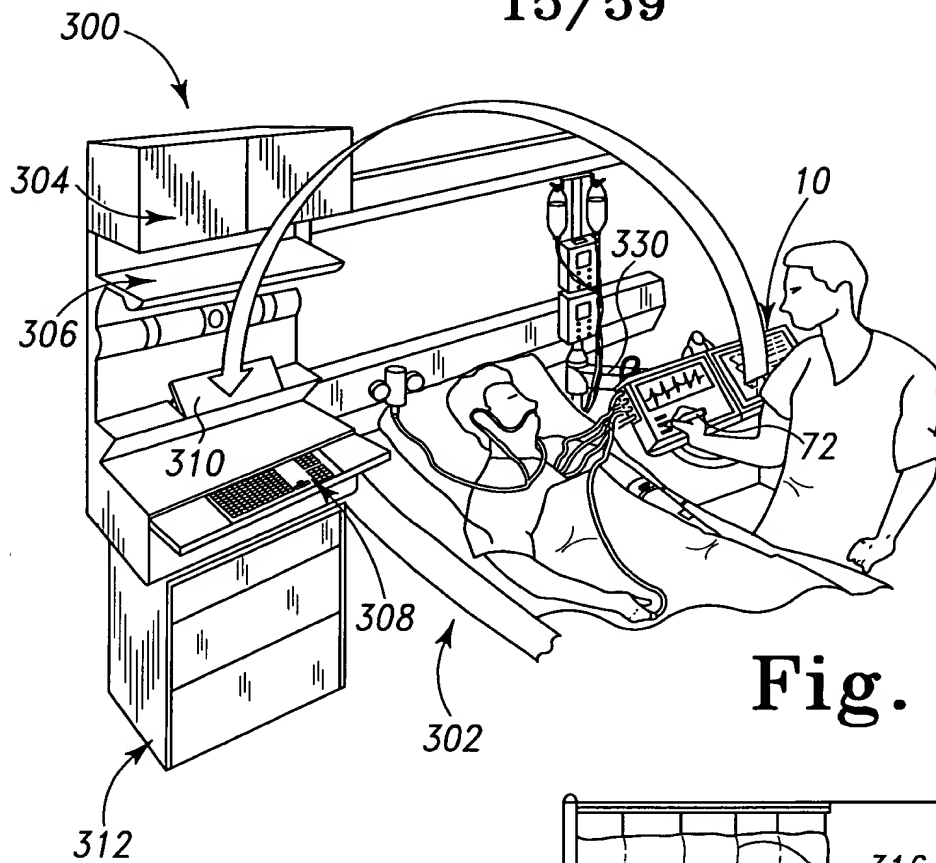


Fig. 25

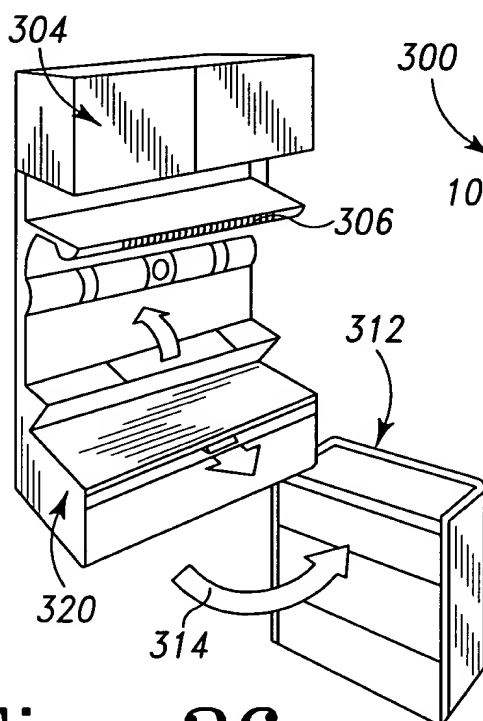


Fig. 26

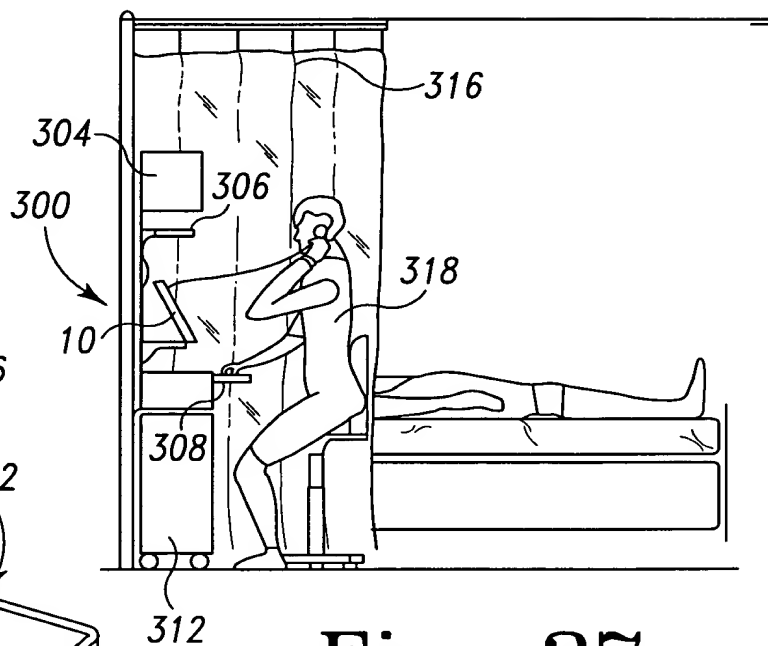


Fig. 27

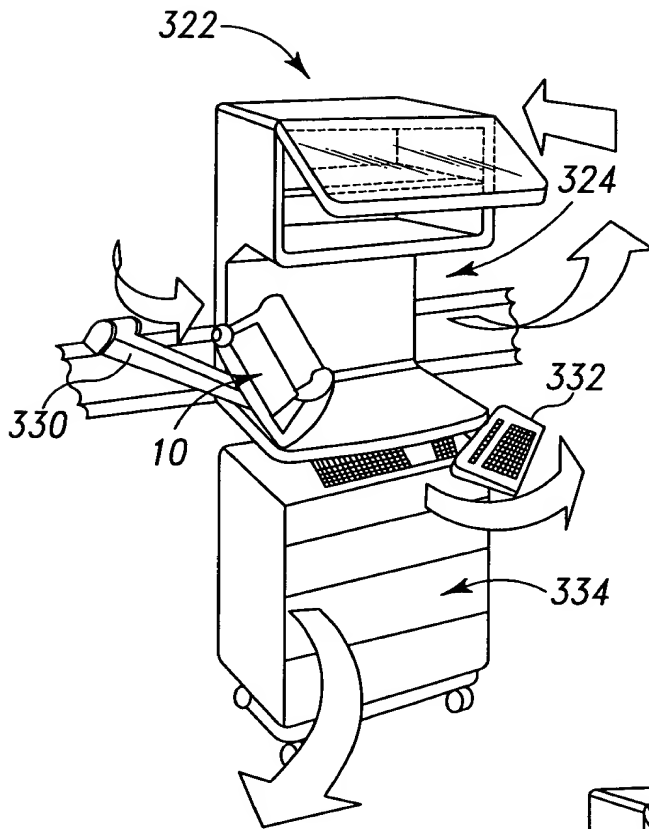


Fig. 29

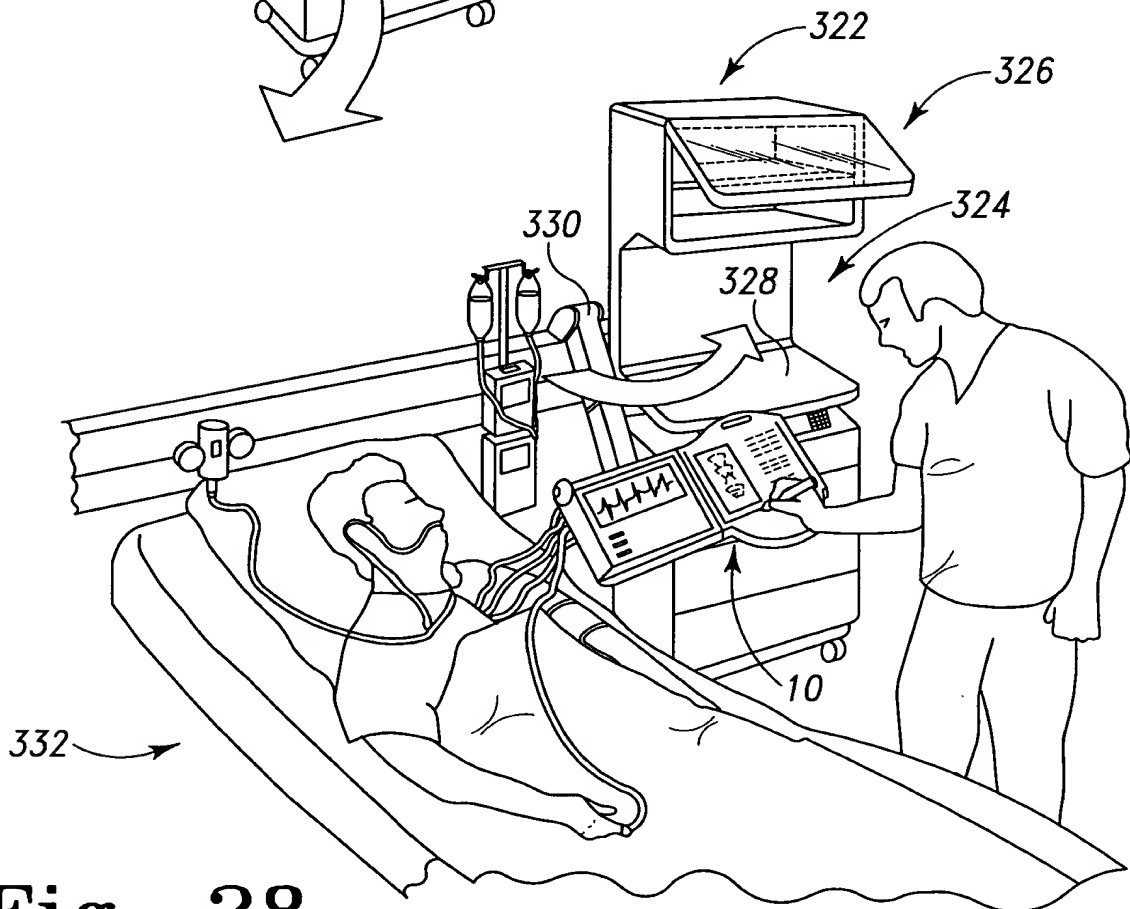


Fig. 28

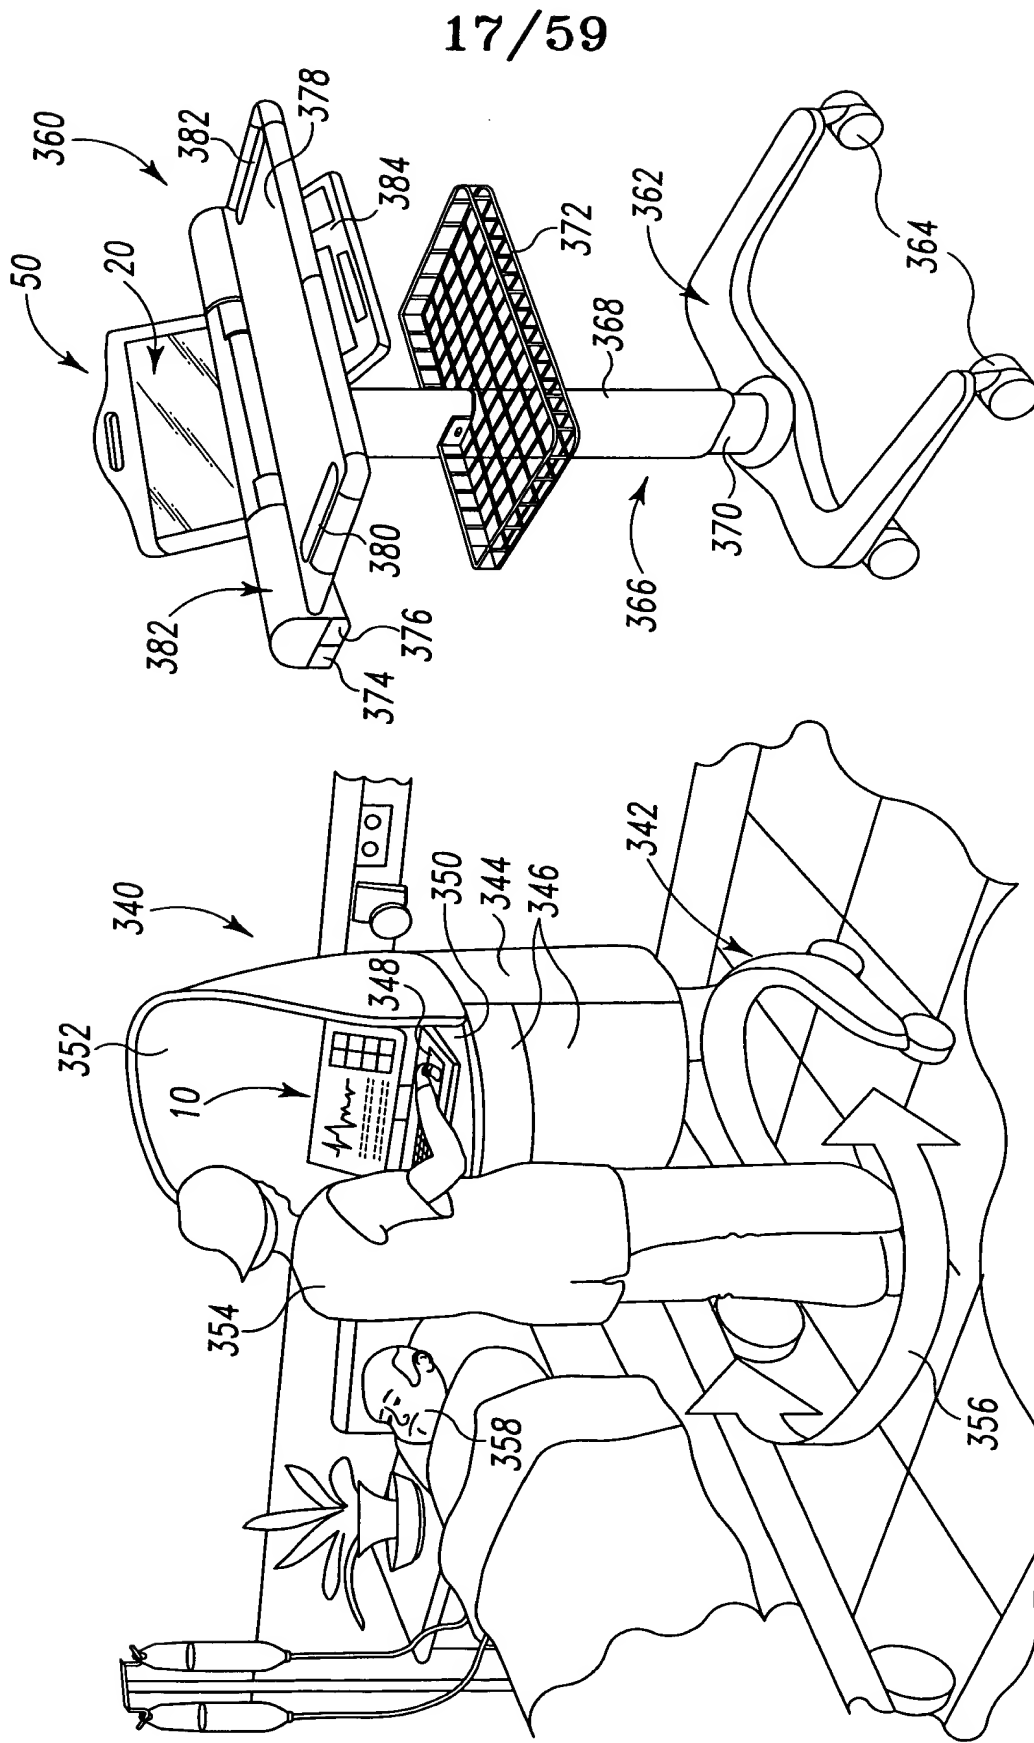


Fig. 30

Fig. 31

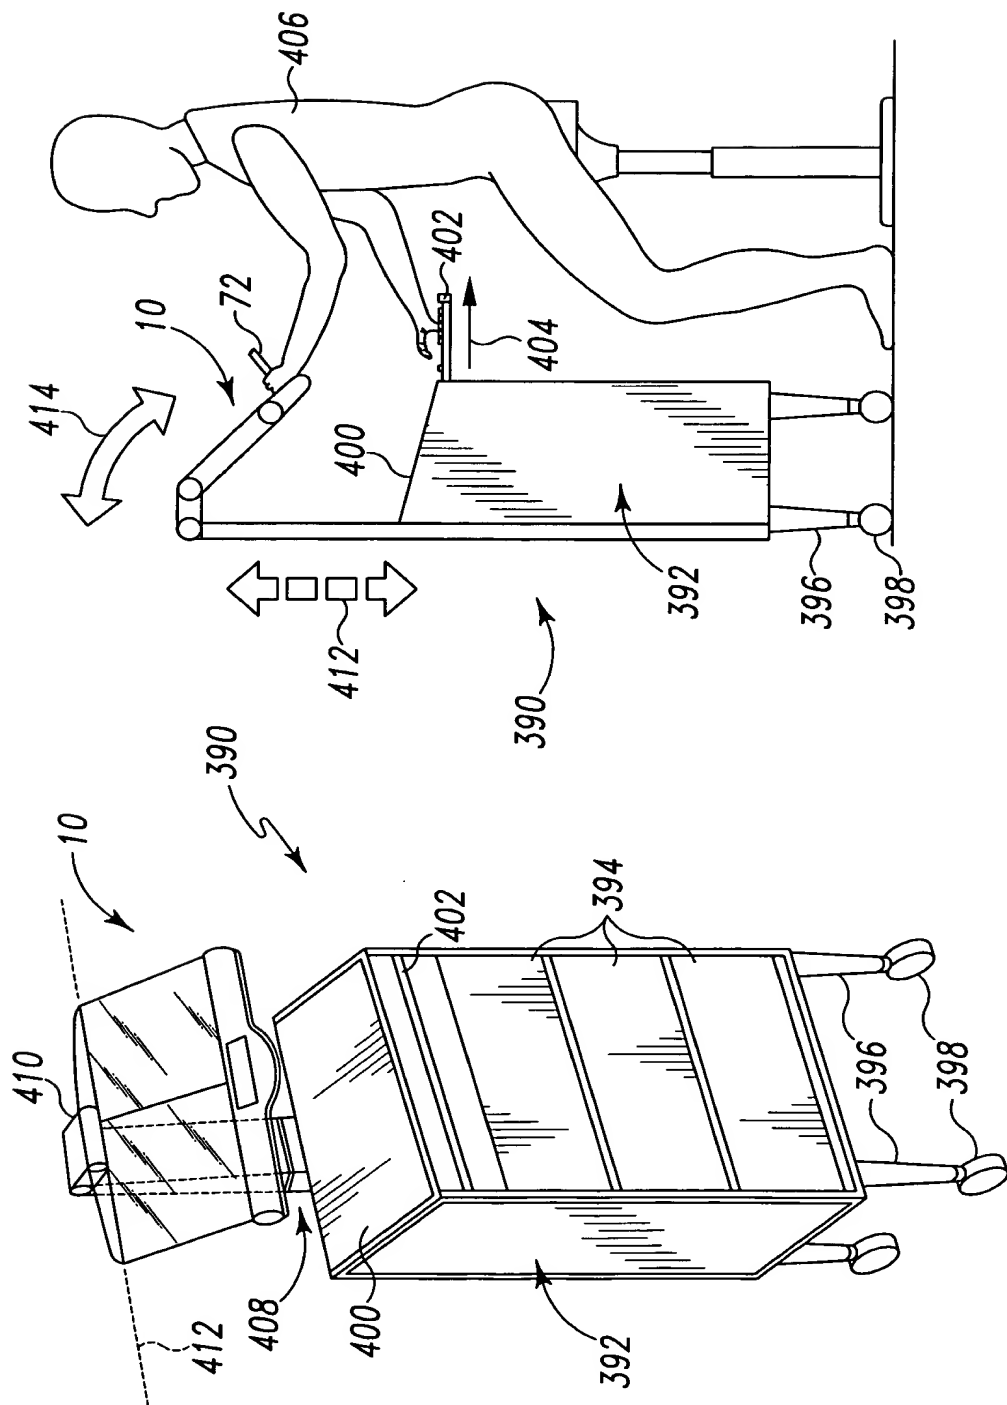


Fig. 33

Fig. 32

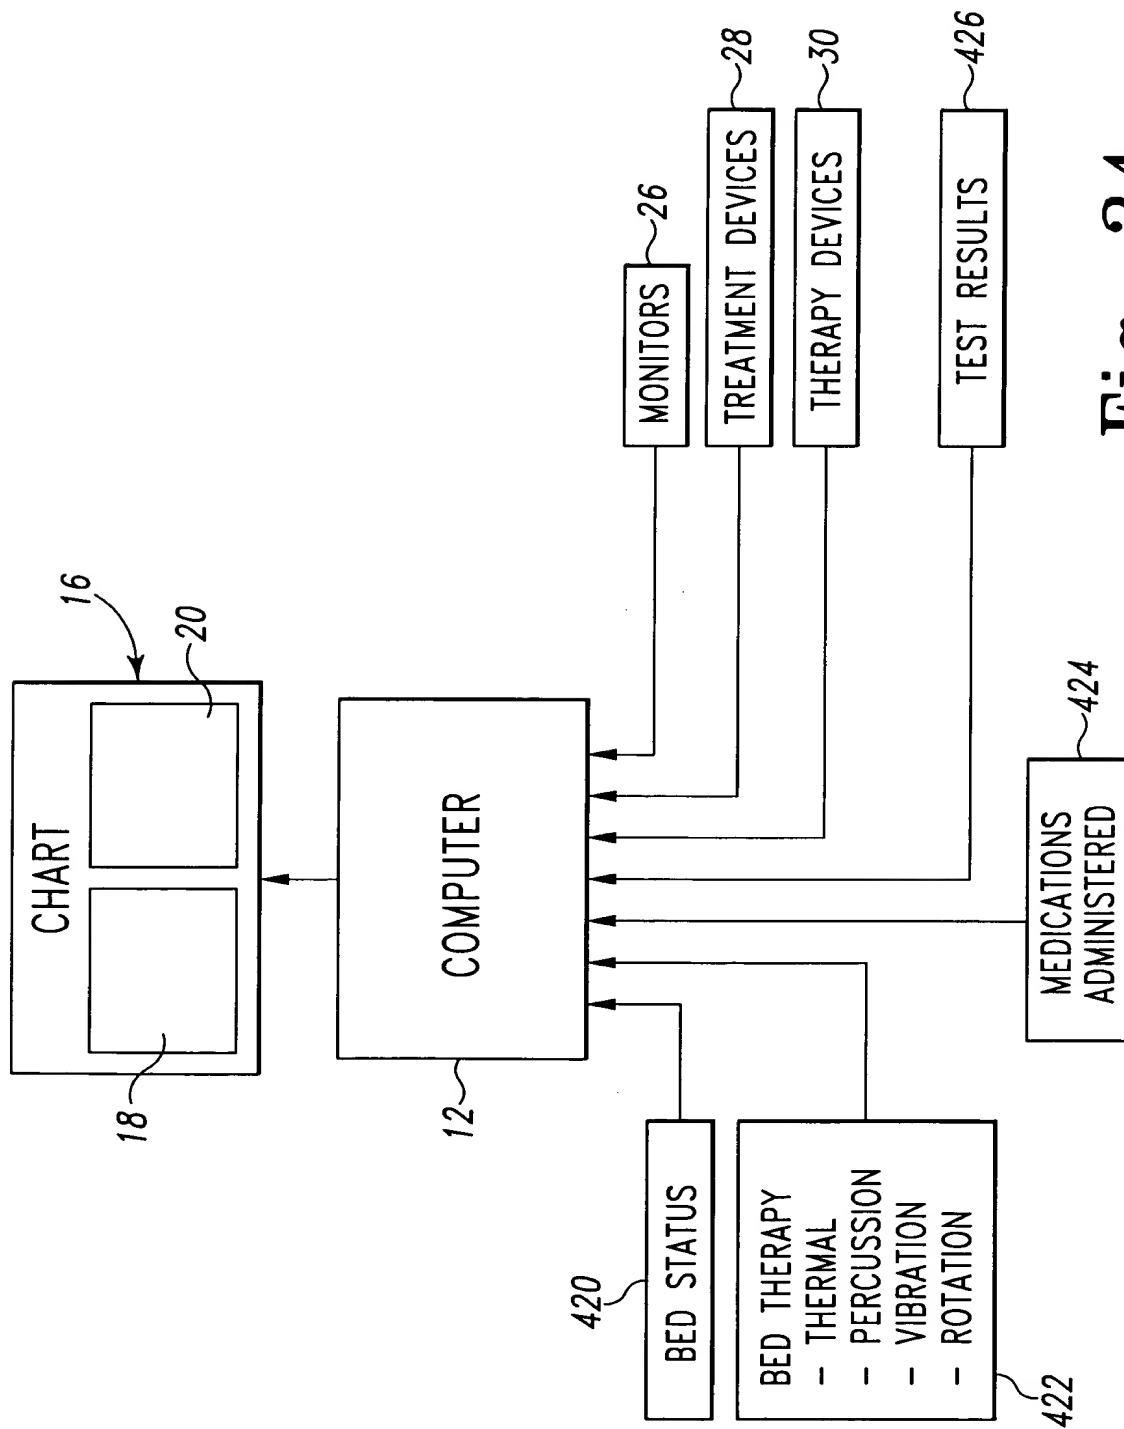


Fig. 34

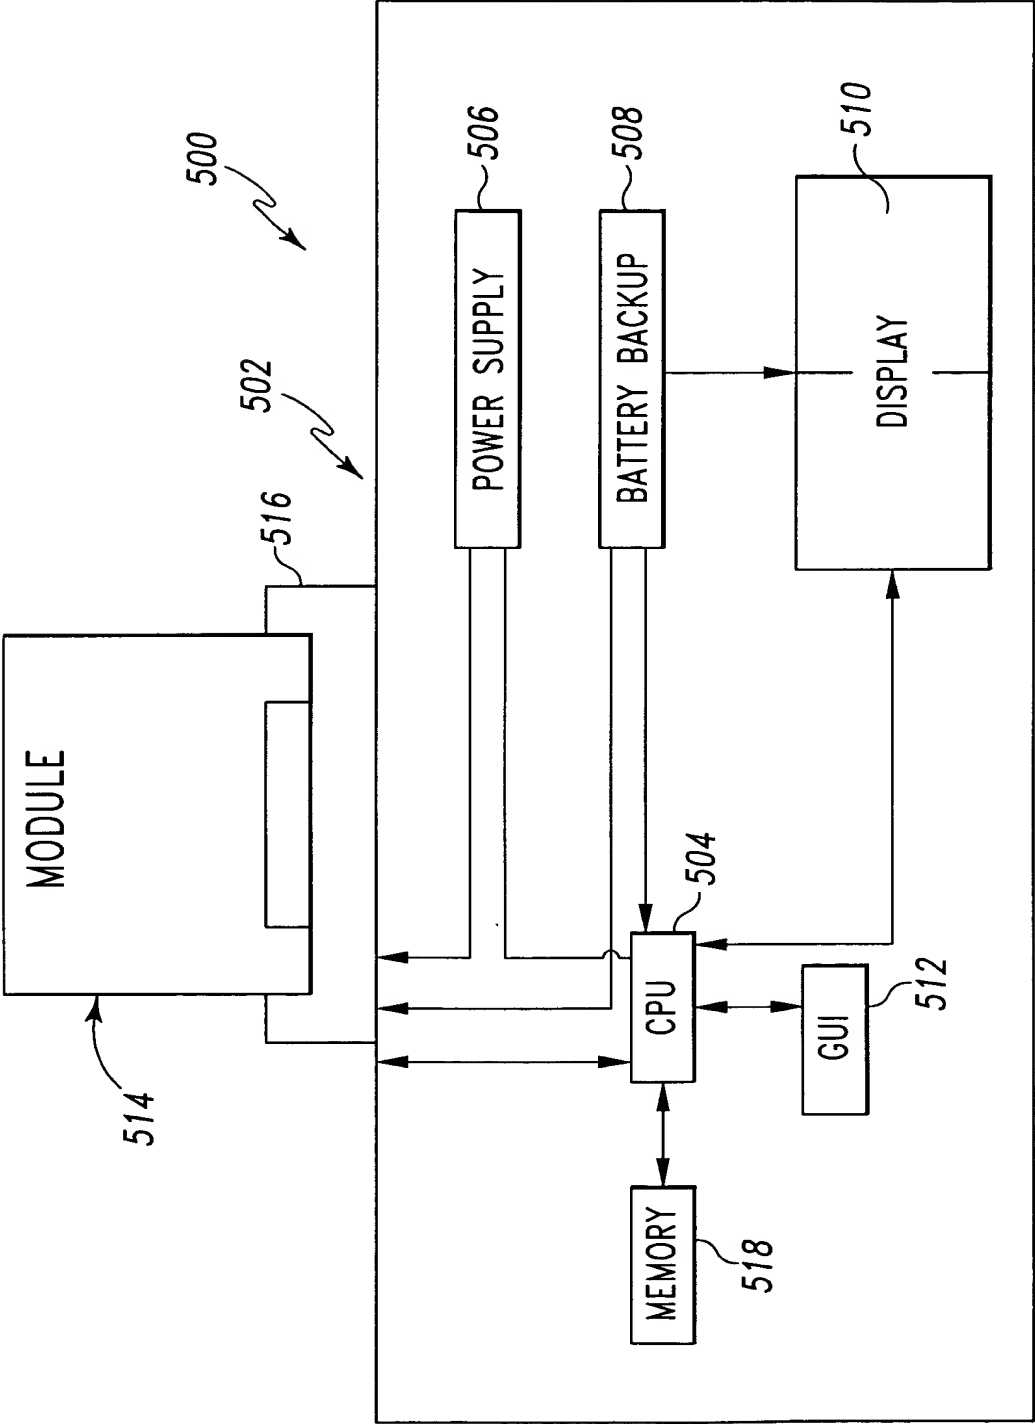


Fig. 35

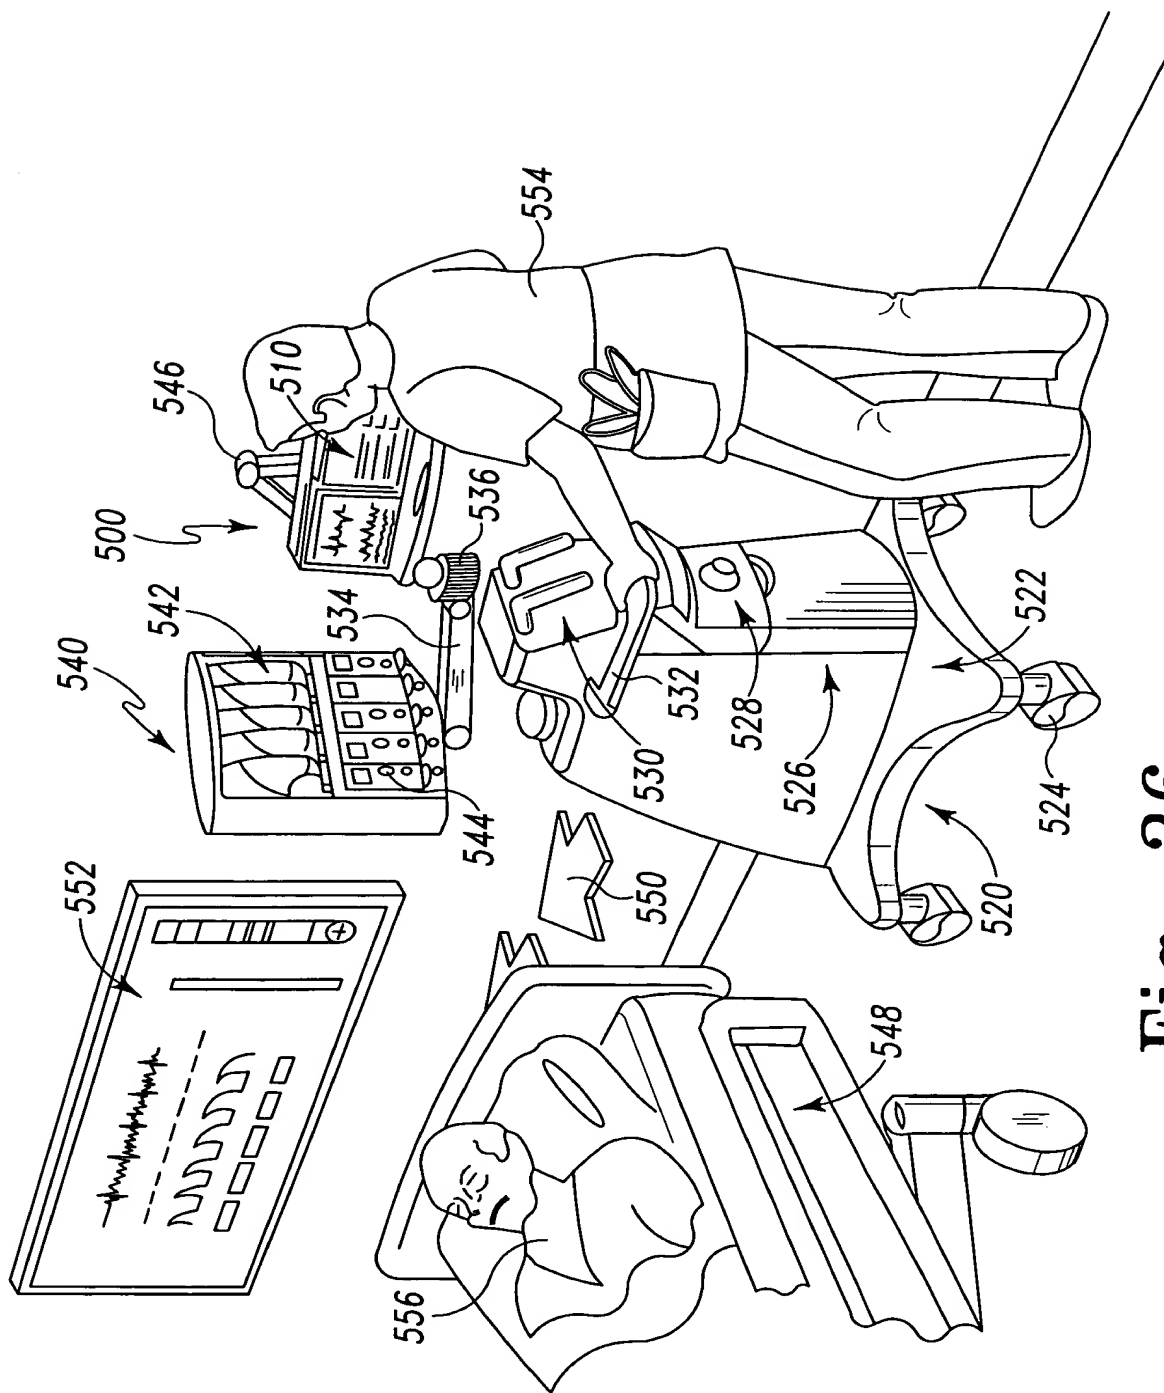


Fig. 36

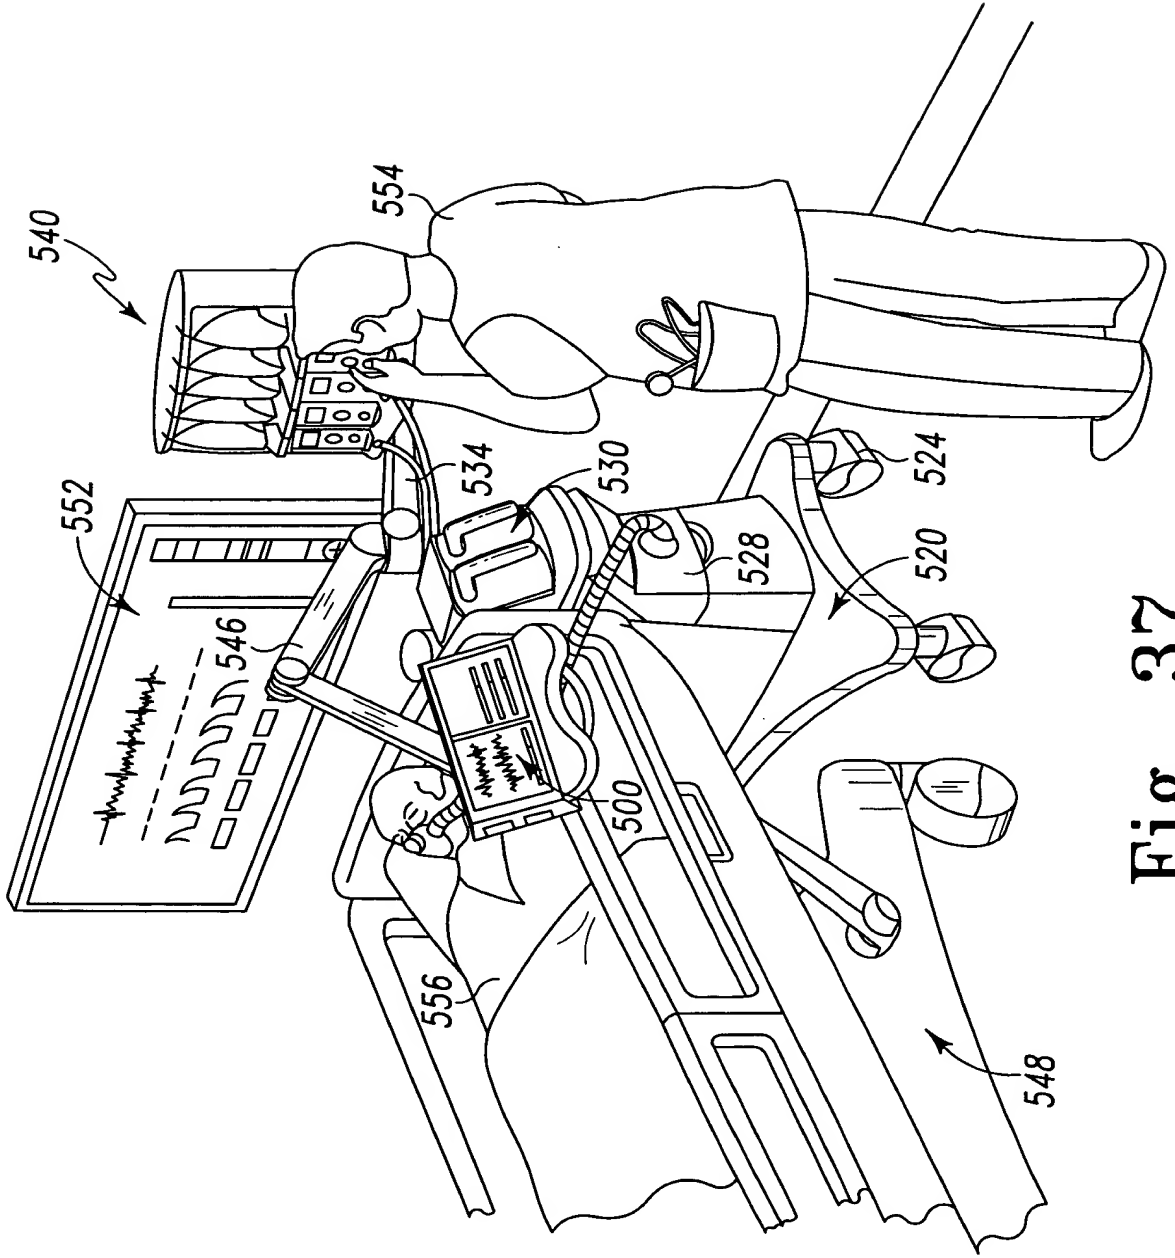
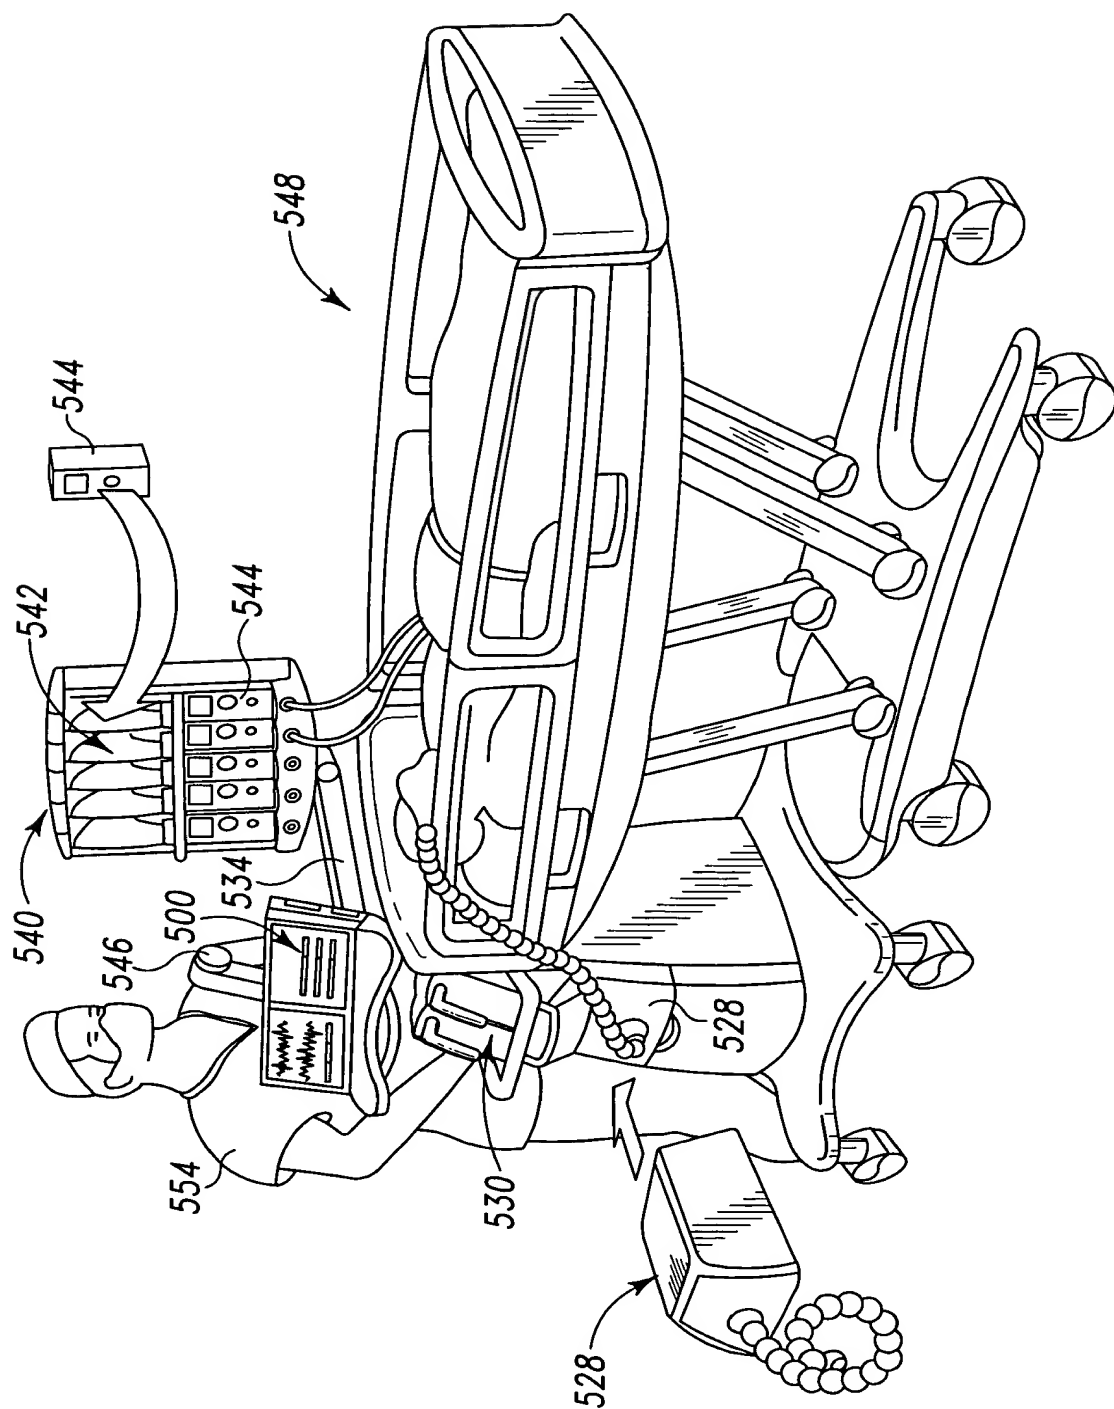


Fig. 37



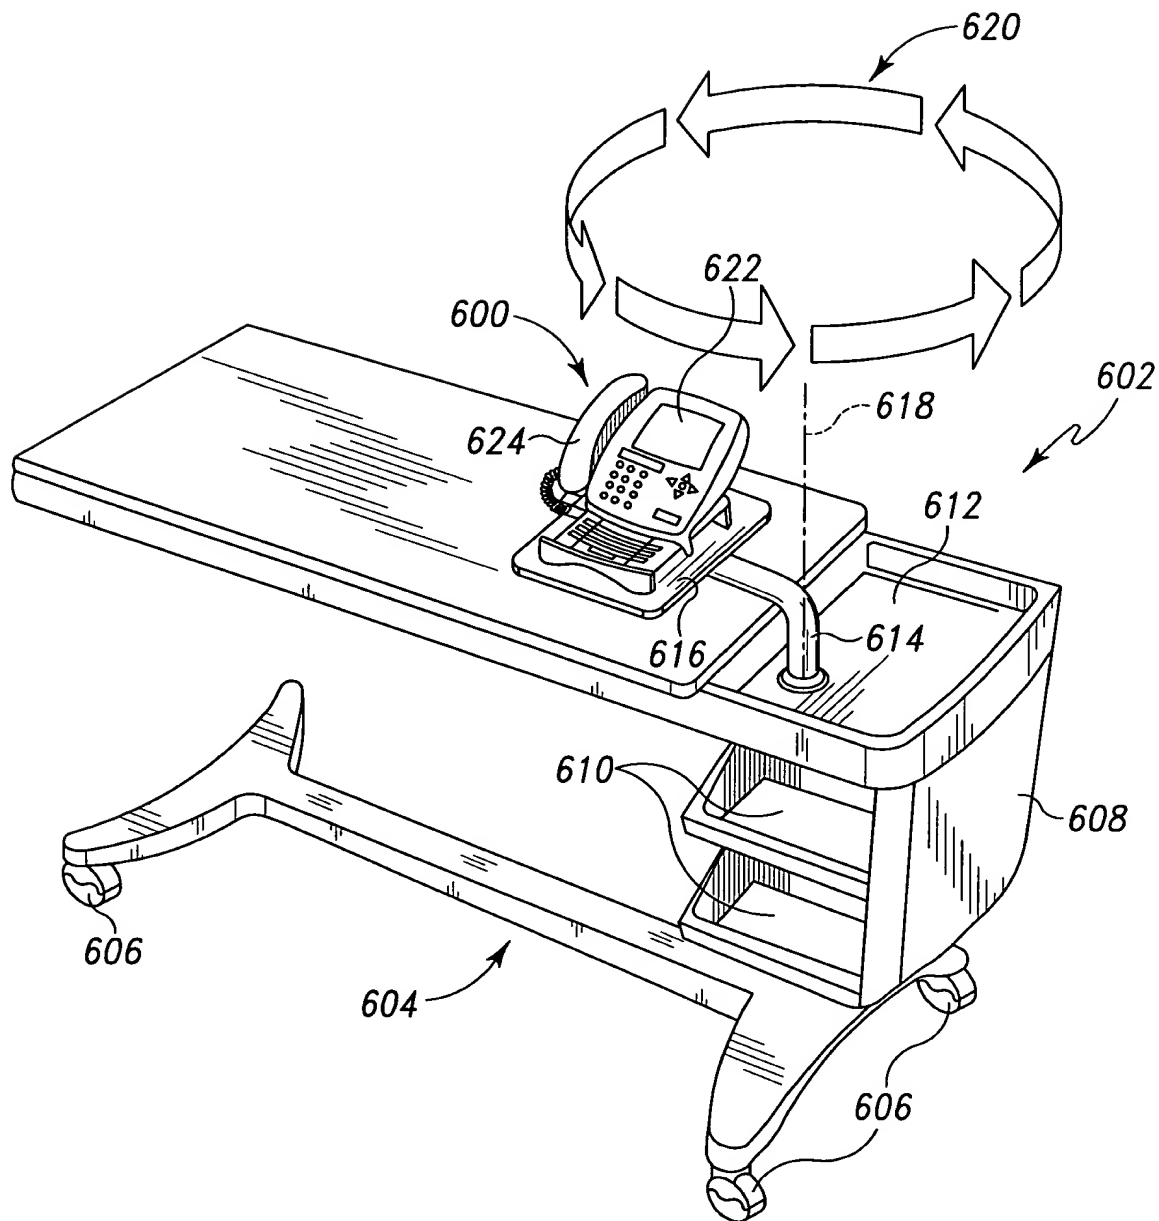


Fig. 39

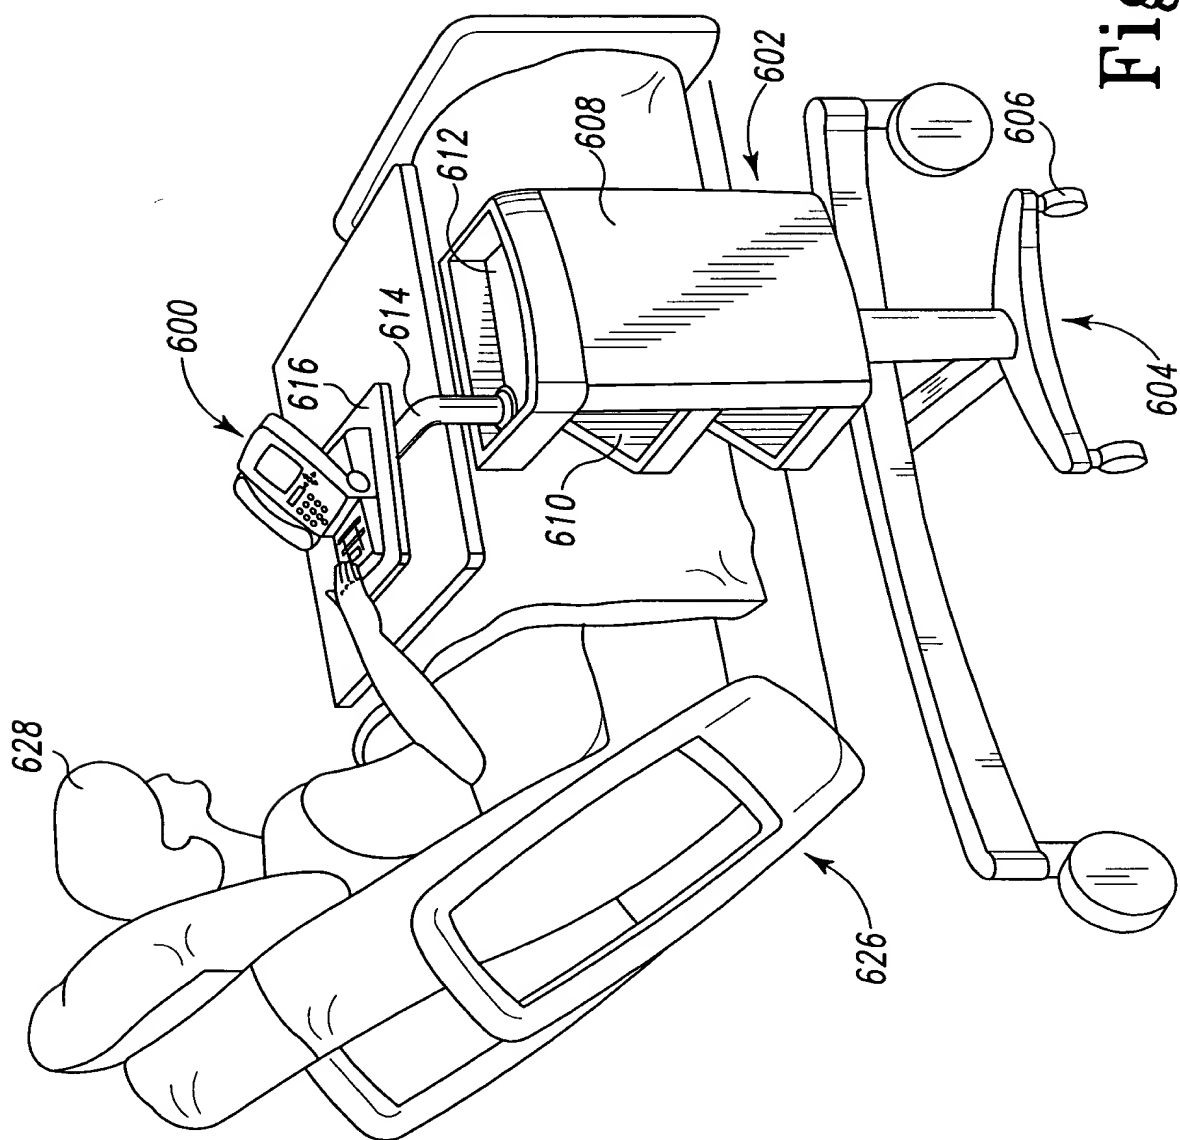


Fig. 40

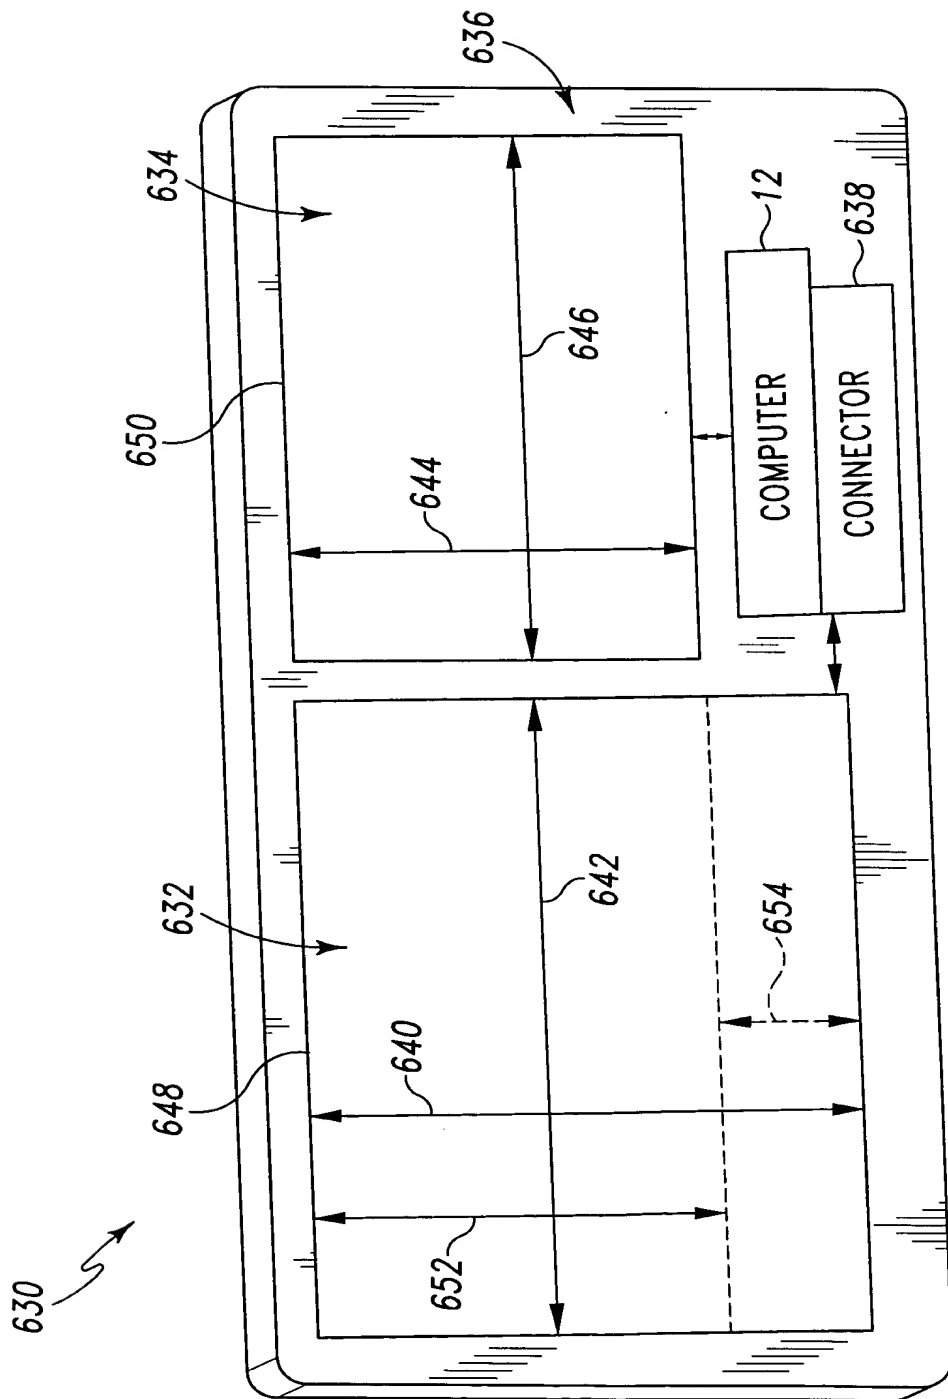


Fig. 41




Fig. 42

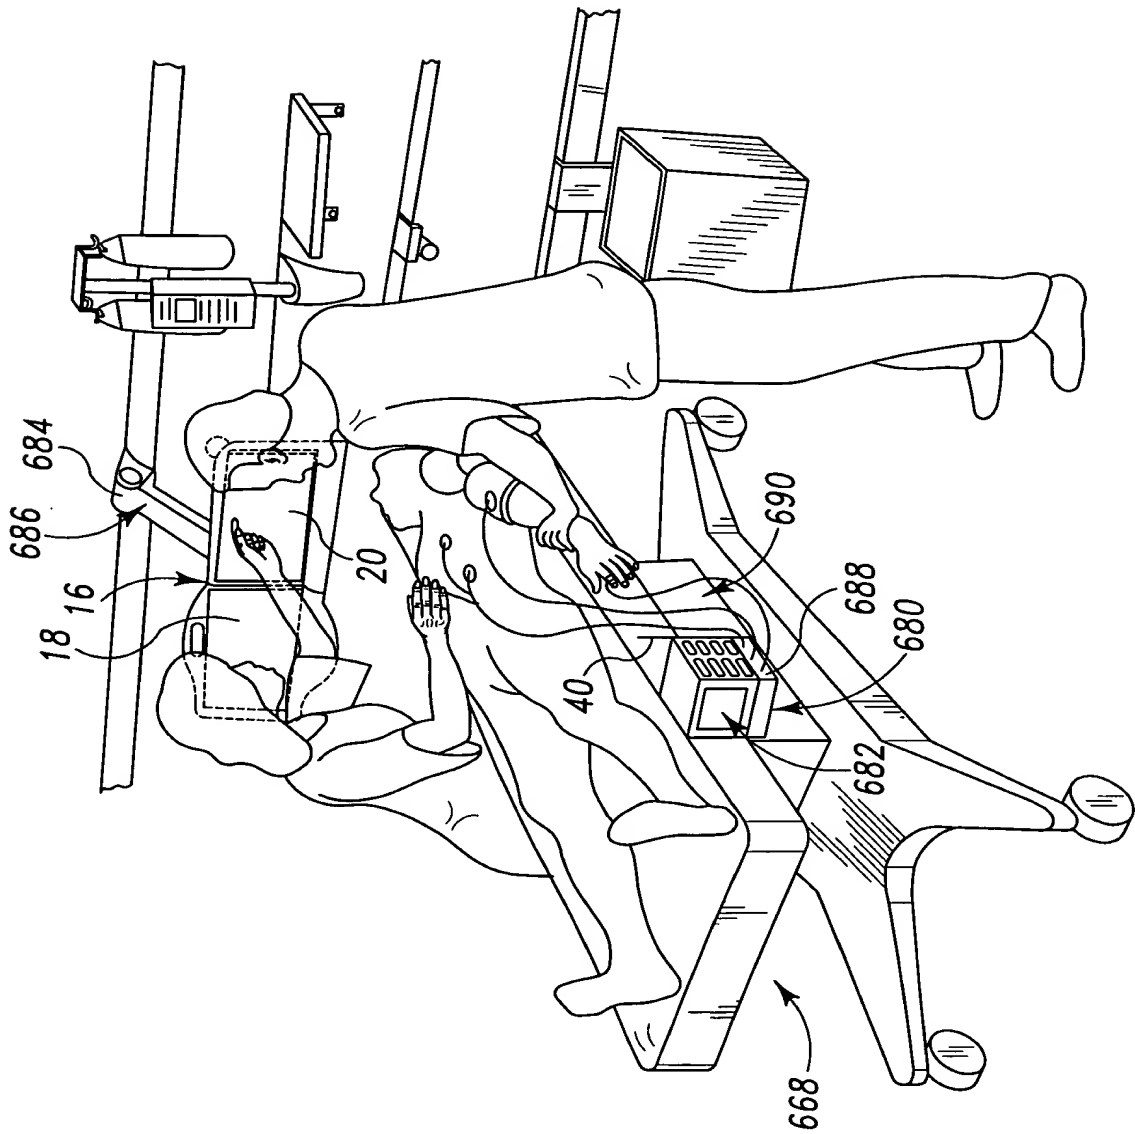


Fig. 43

29/59

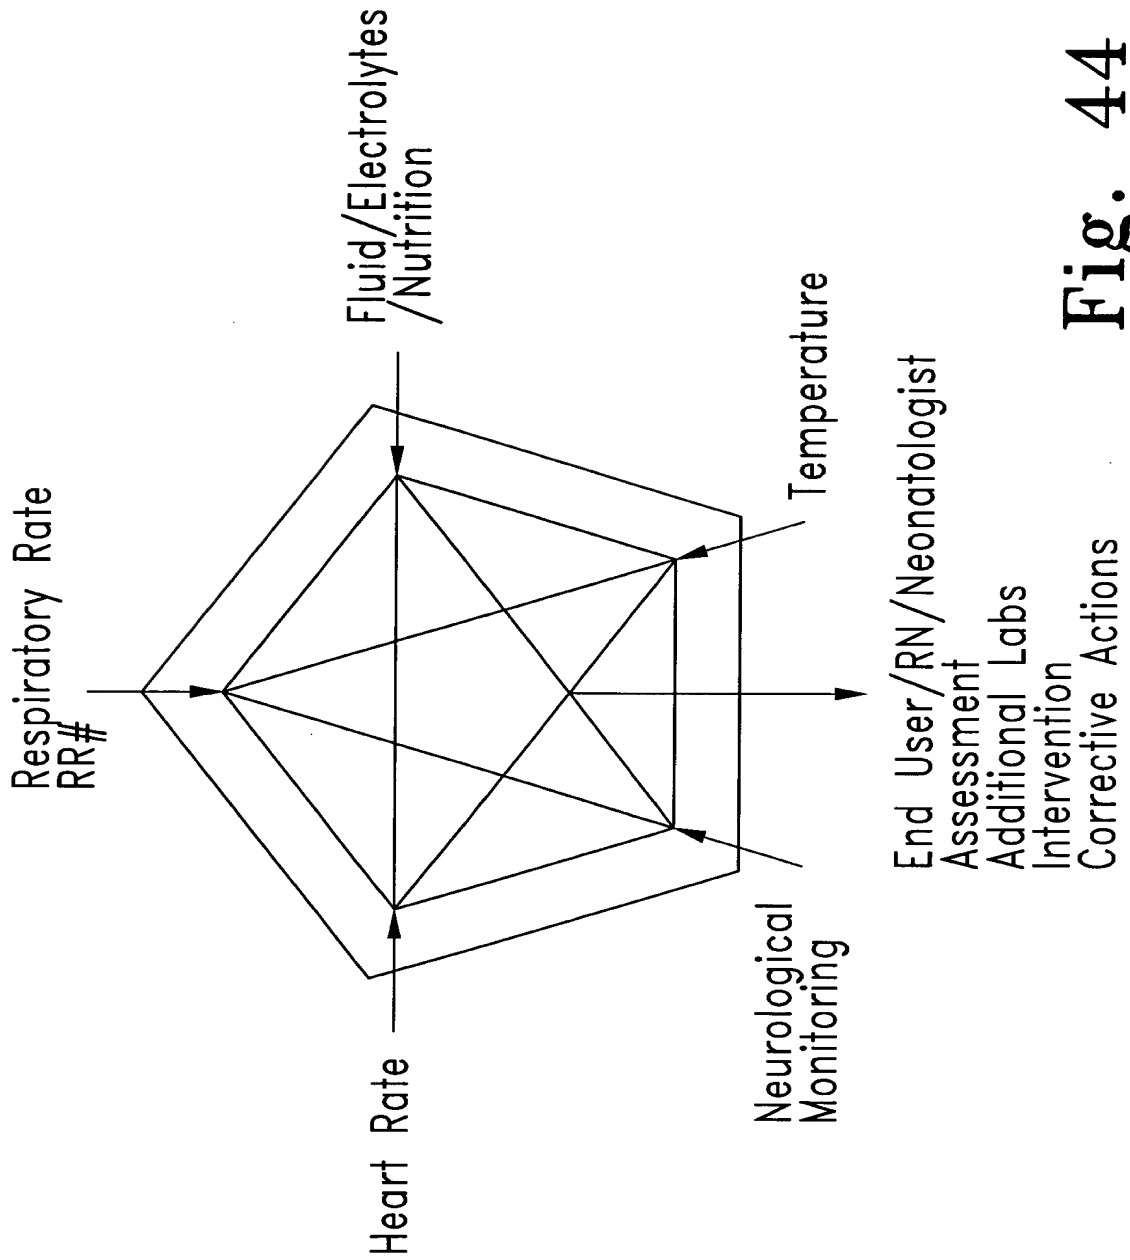


Fig. 44

30/59

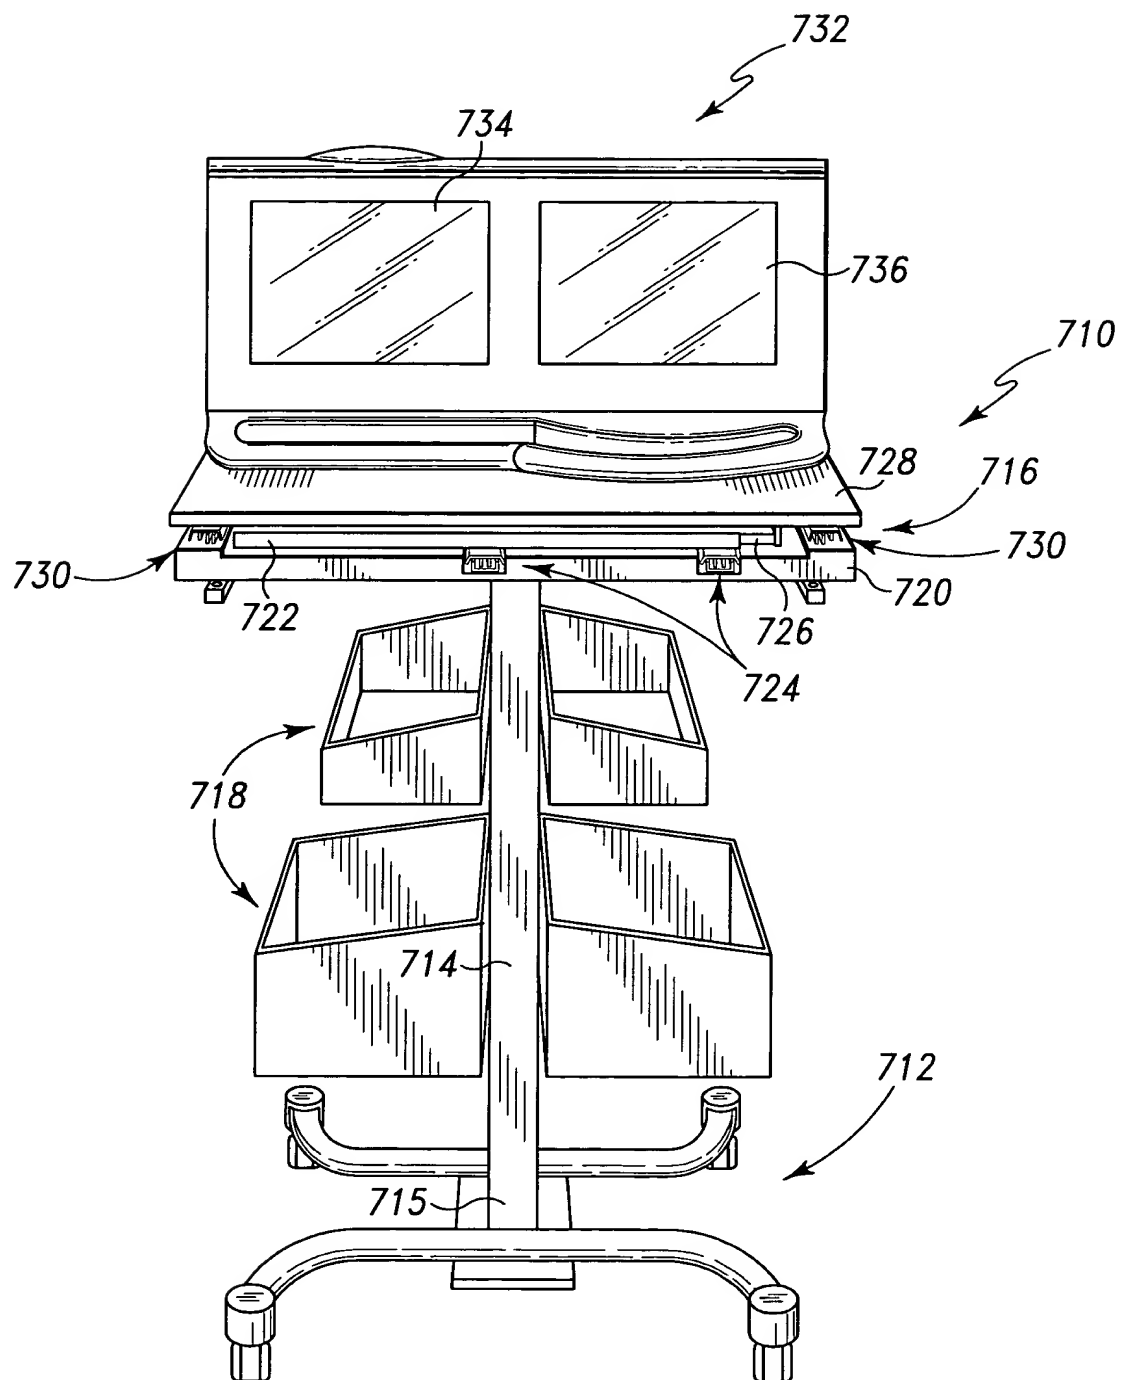


Fig. 45

09849580-121301

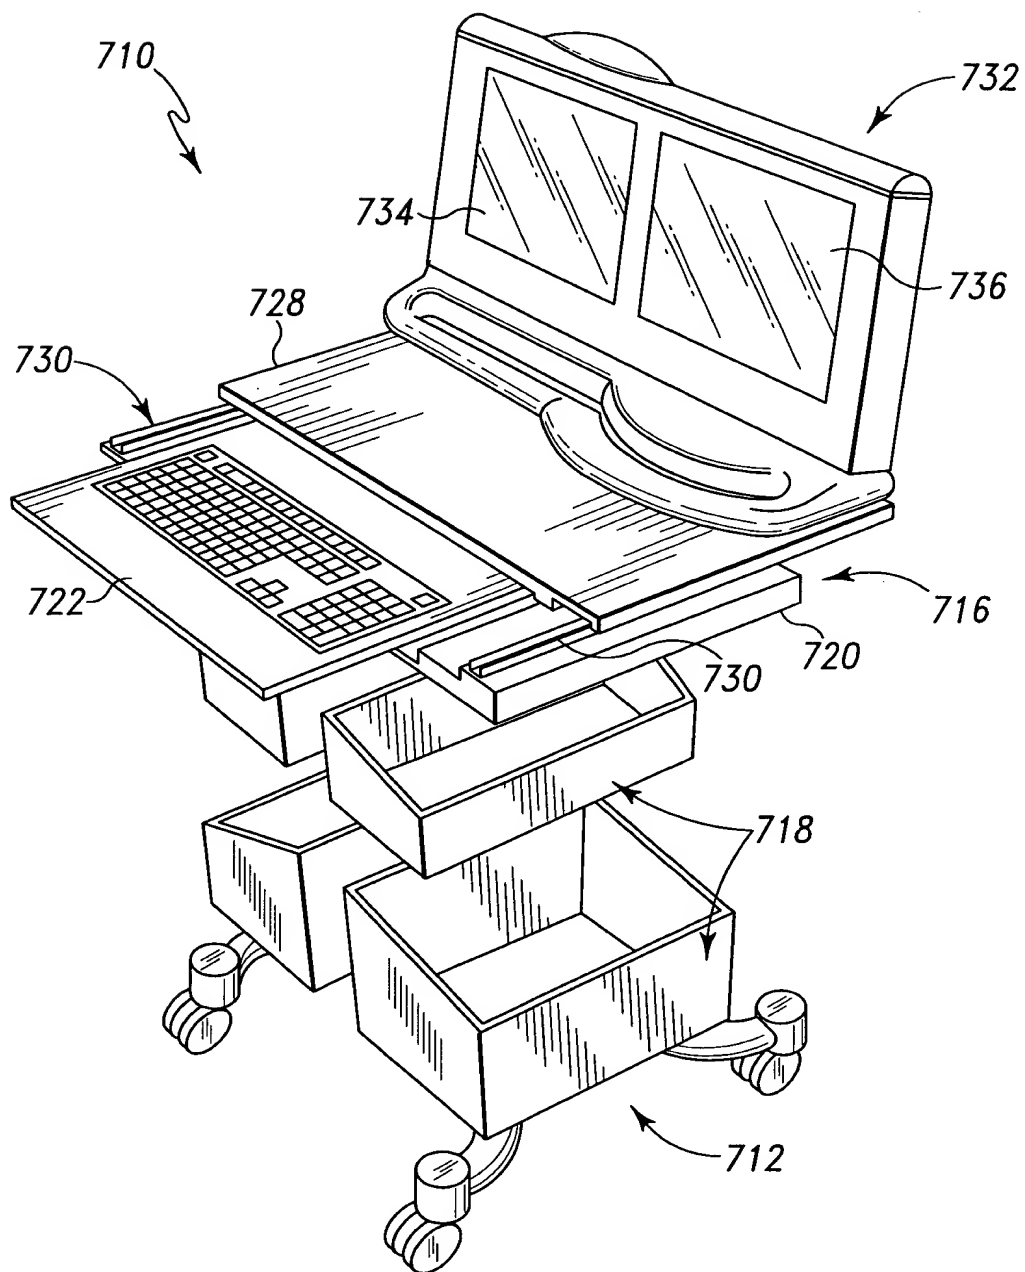


Fig. 46

JOHN SMITH		<input checked="" type="checkbox"/>	6/24/00		11:05								
VITALS		TRENDS		P.INFO		SET-UP		HISTORY		EQUIP.		CPR	
TIME		10:00		11:00		12:00		1:00		2:00			
CORE TEMP		39.2		39.2		39.2		39.2		39.2			
HEART RATE		107		108		107		107		107			
HEART RHYTHM		S TACH		S TACH		S TACH		S TACH		S TACH			
ART SYSTOLIC		150		160		150		150		150			
ART DIASTOLIC		90		94		90		90		90			
ART MEAN		110		116		110		110		110			
PA SYSTOLIC		43		54		43		43		43			
PA DIASTOLIC		22		25		22		22		22			
PA MEAN		30		30		30		30		30			
PCMP		20		10		20		20		20			
CVP		10		10		10		10		10			
CO		4.70		4.70		4.70		4.70		4.70			
CI		2.17		2.17		2.17		2.17		2.17			
SVR		10.89		10.89		10.89		10.89		10.89			
PVR		159		159		159		159		159			
SV02		61		64		61		61		61			
RESPIRATORY RATE		15		11		15		15		15			
SP02		100		99		100		100		100			

Fig. 47A

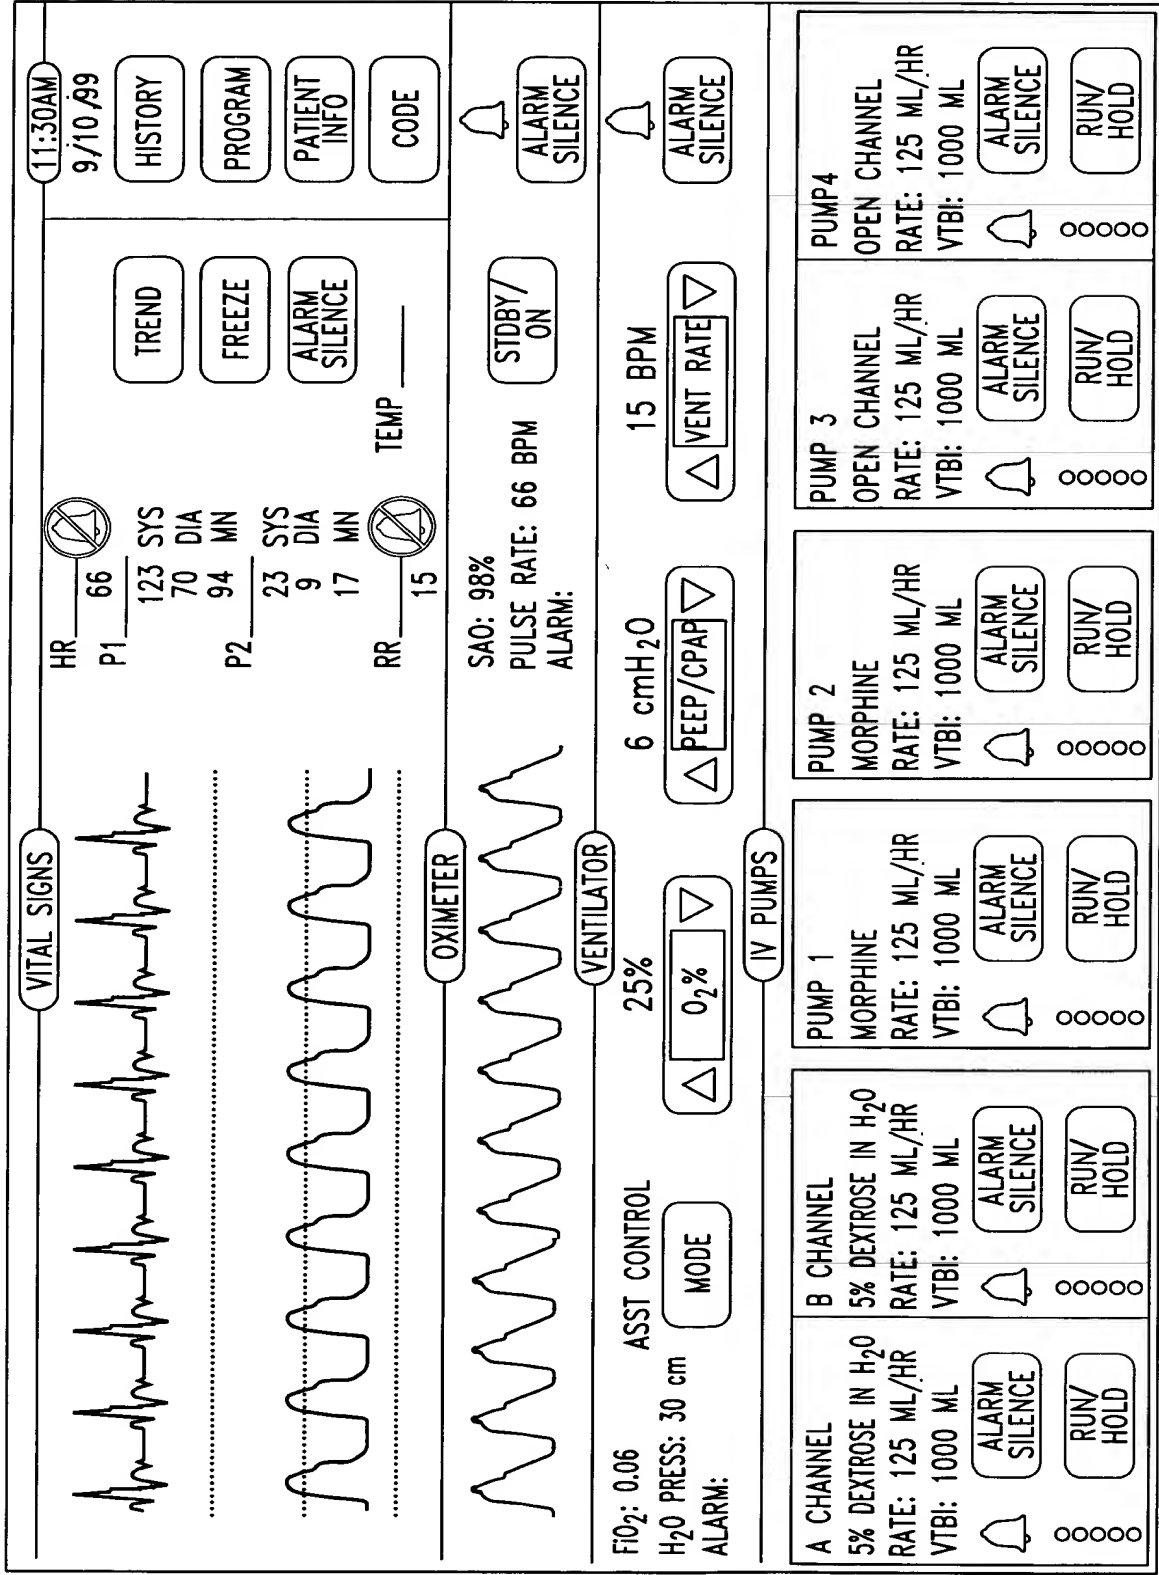


Fig. 48

35/59




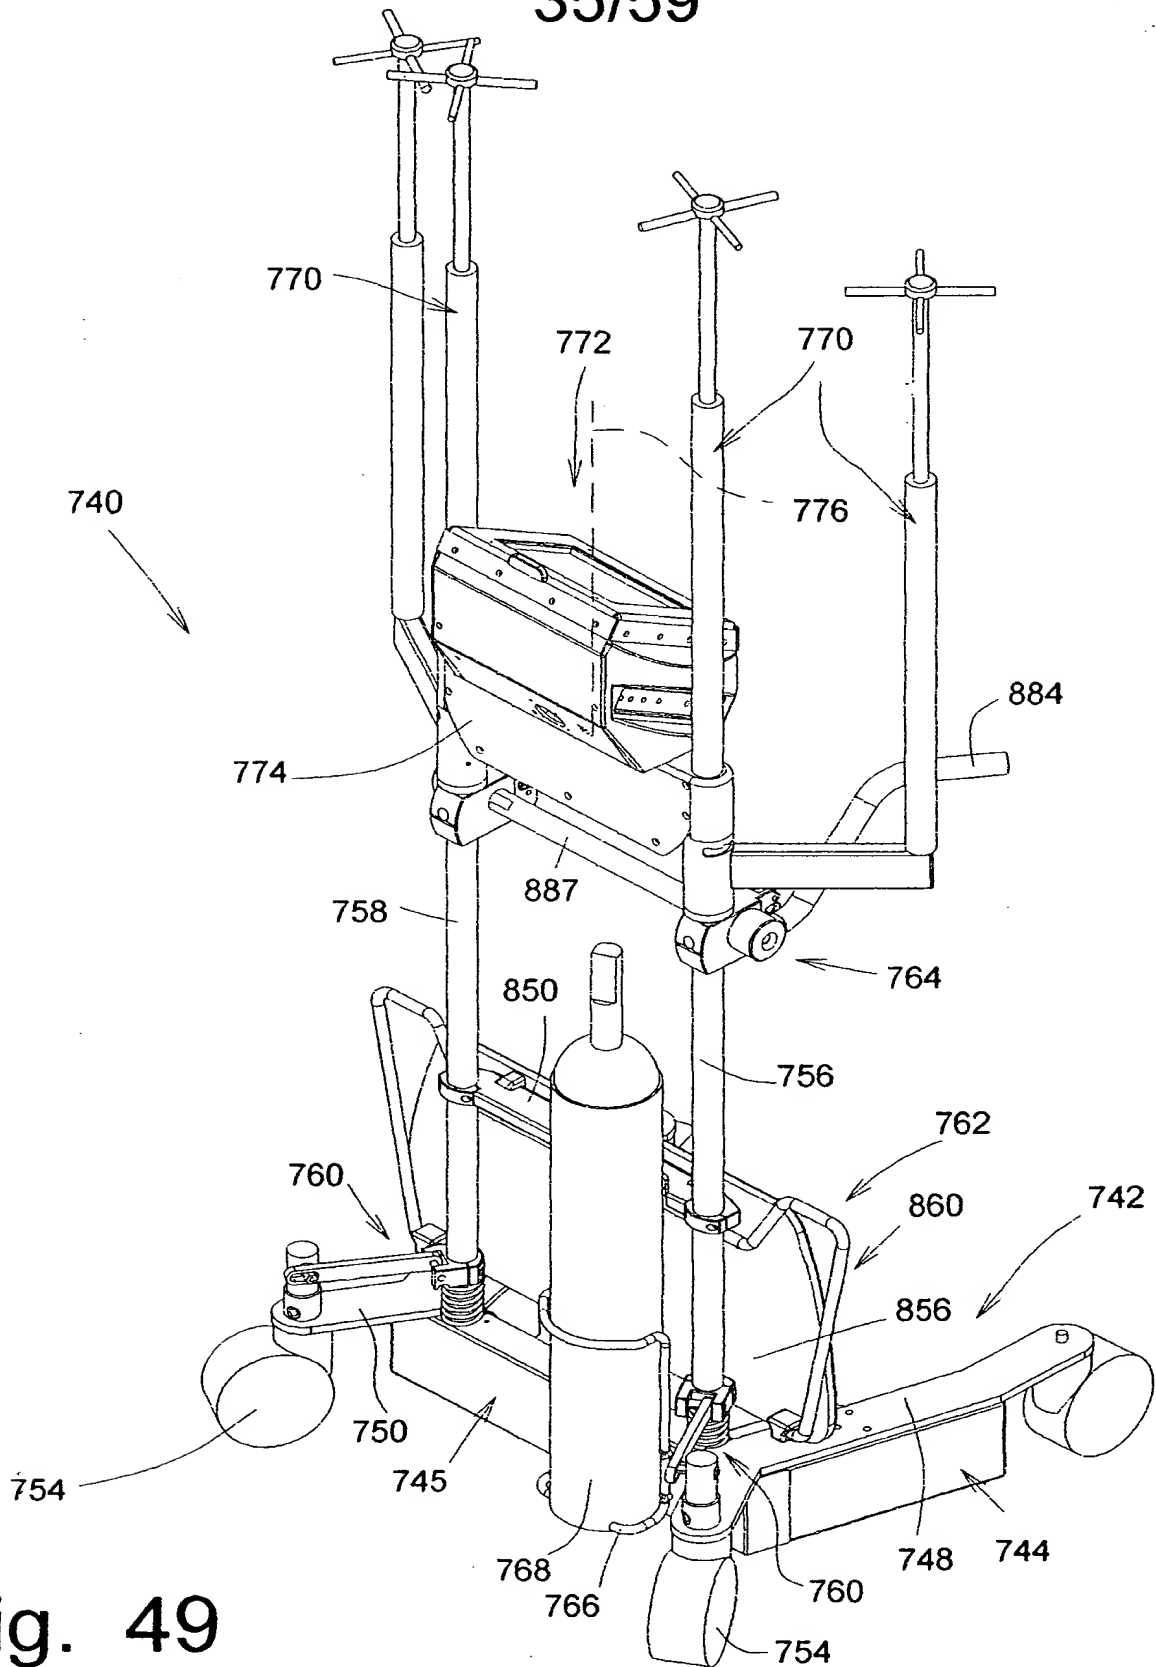


Fig. 49

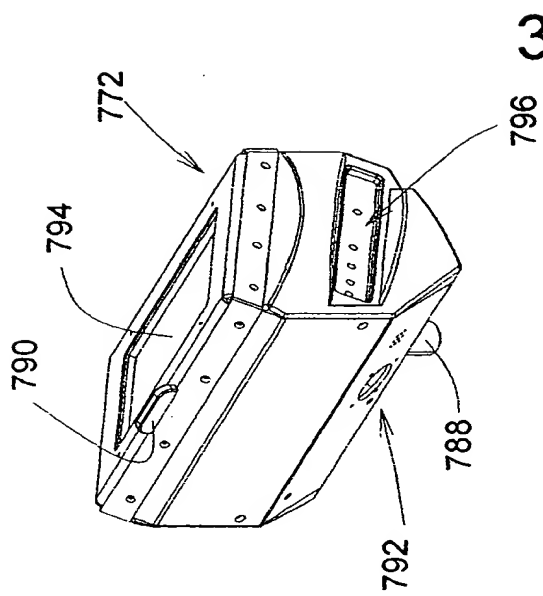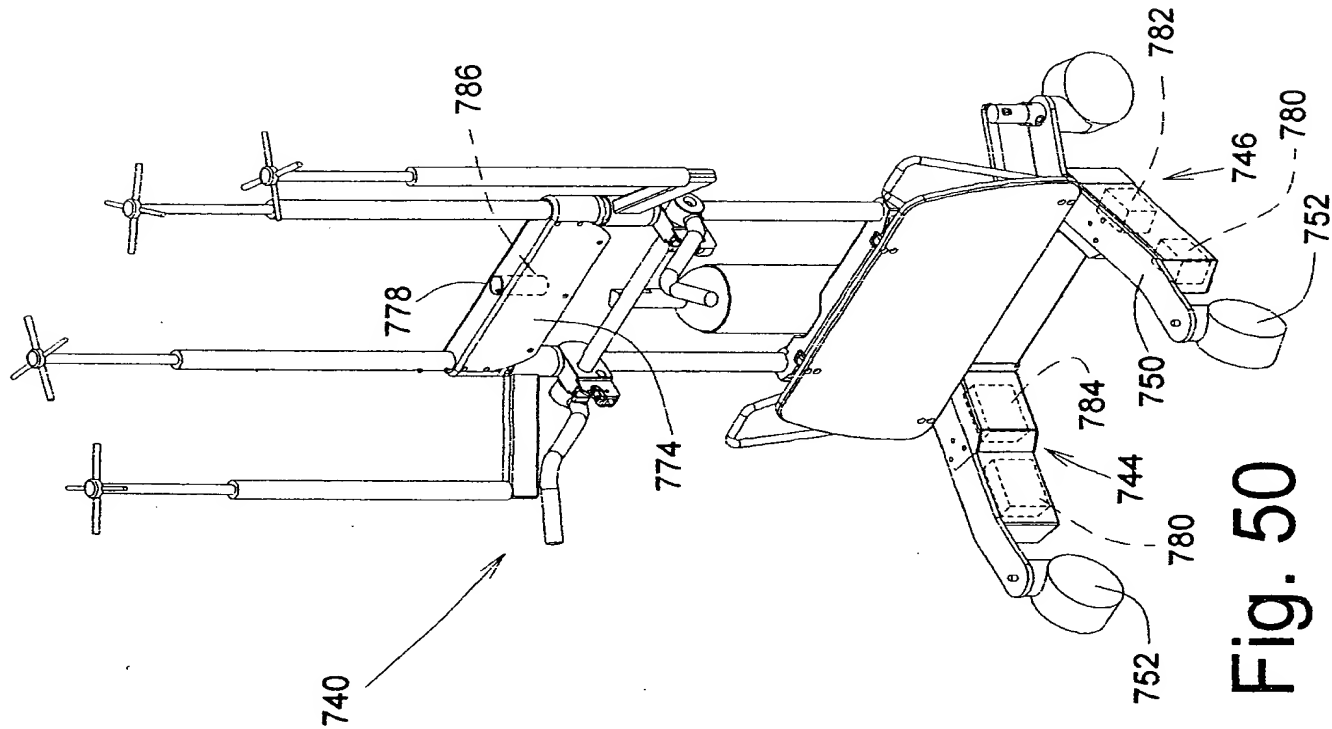

36/59

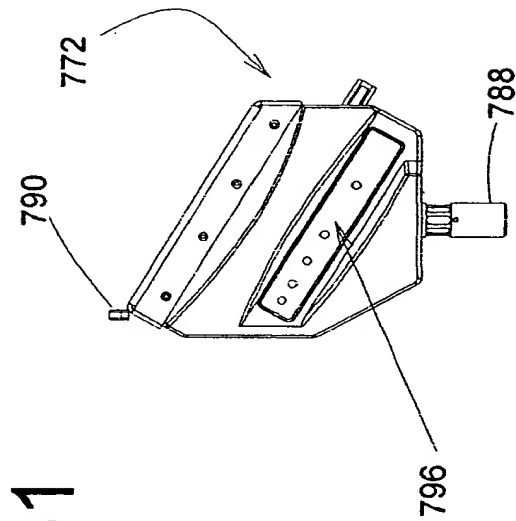

37/59

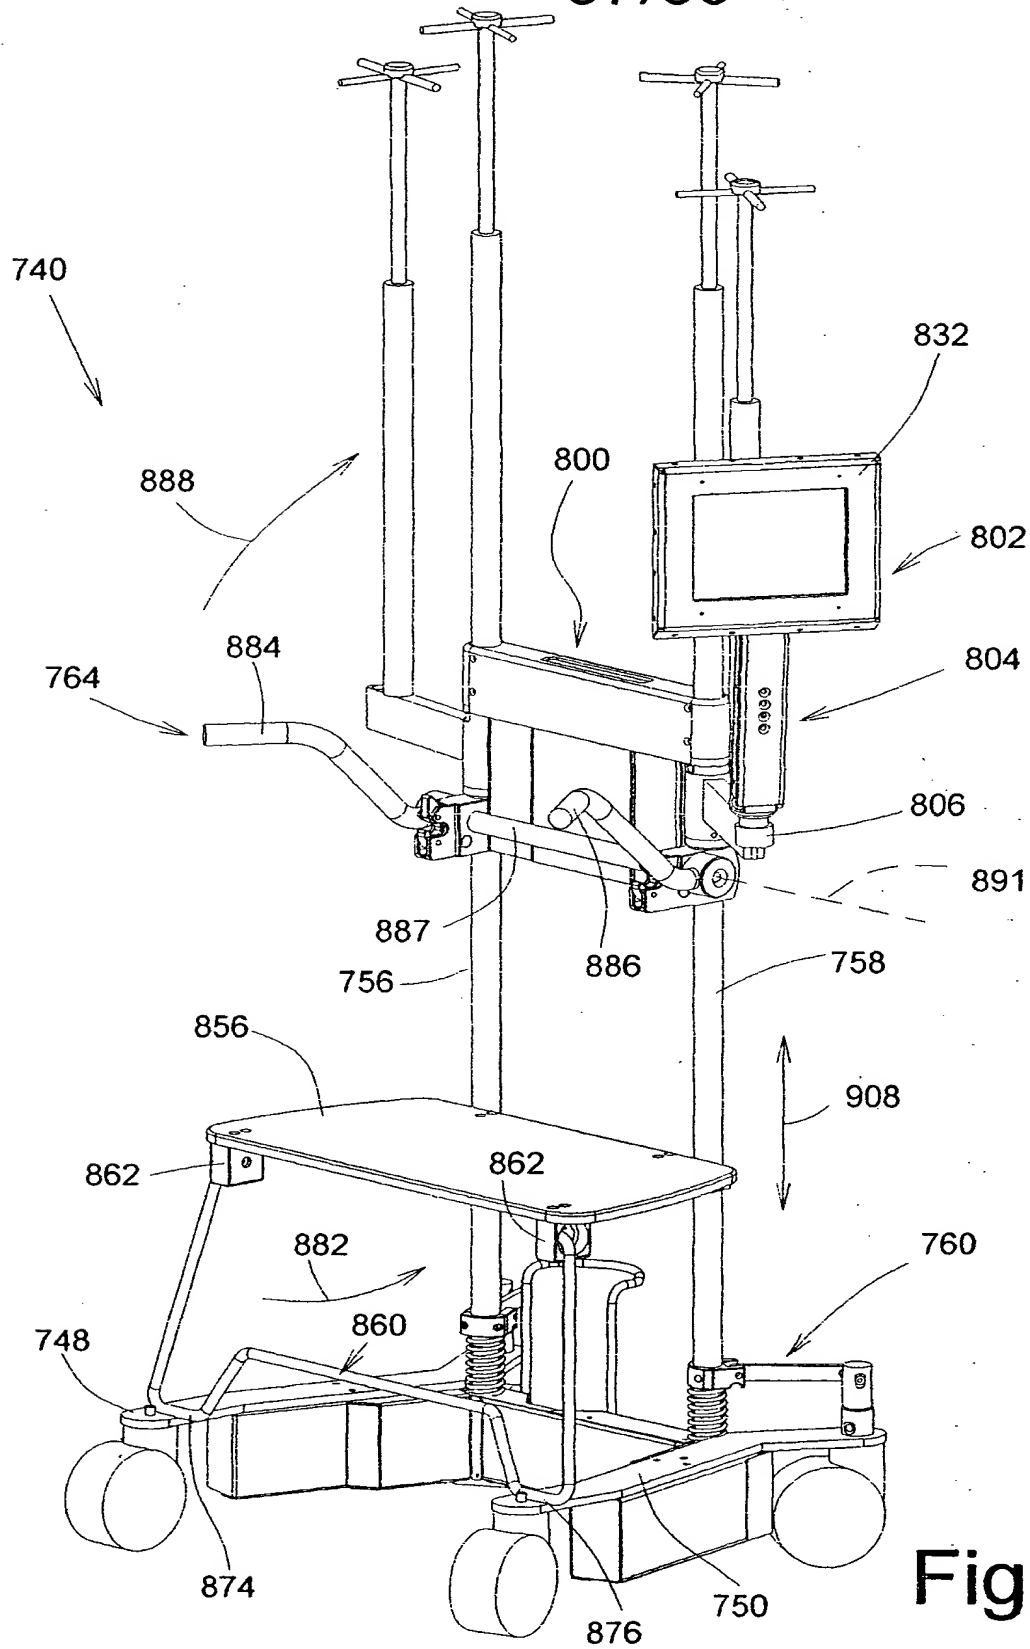


Fig. 53

38/59

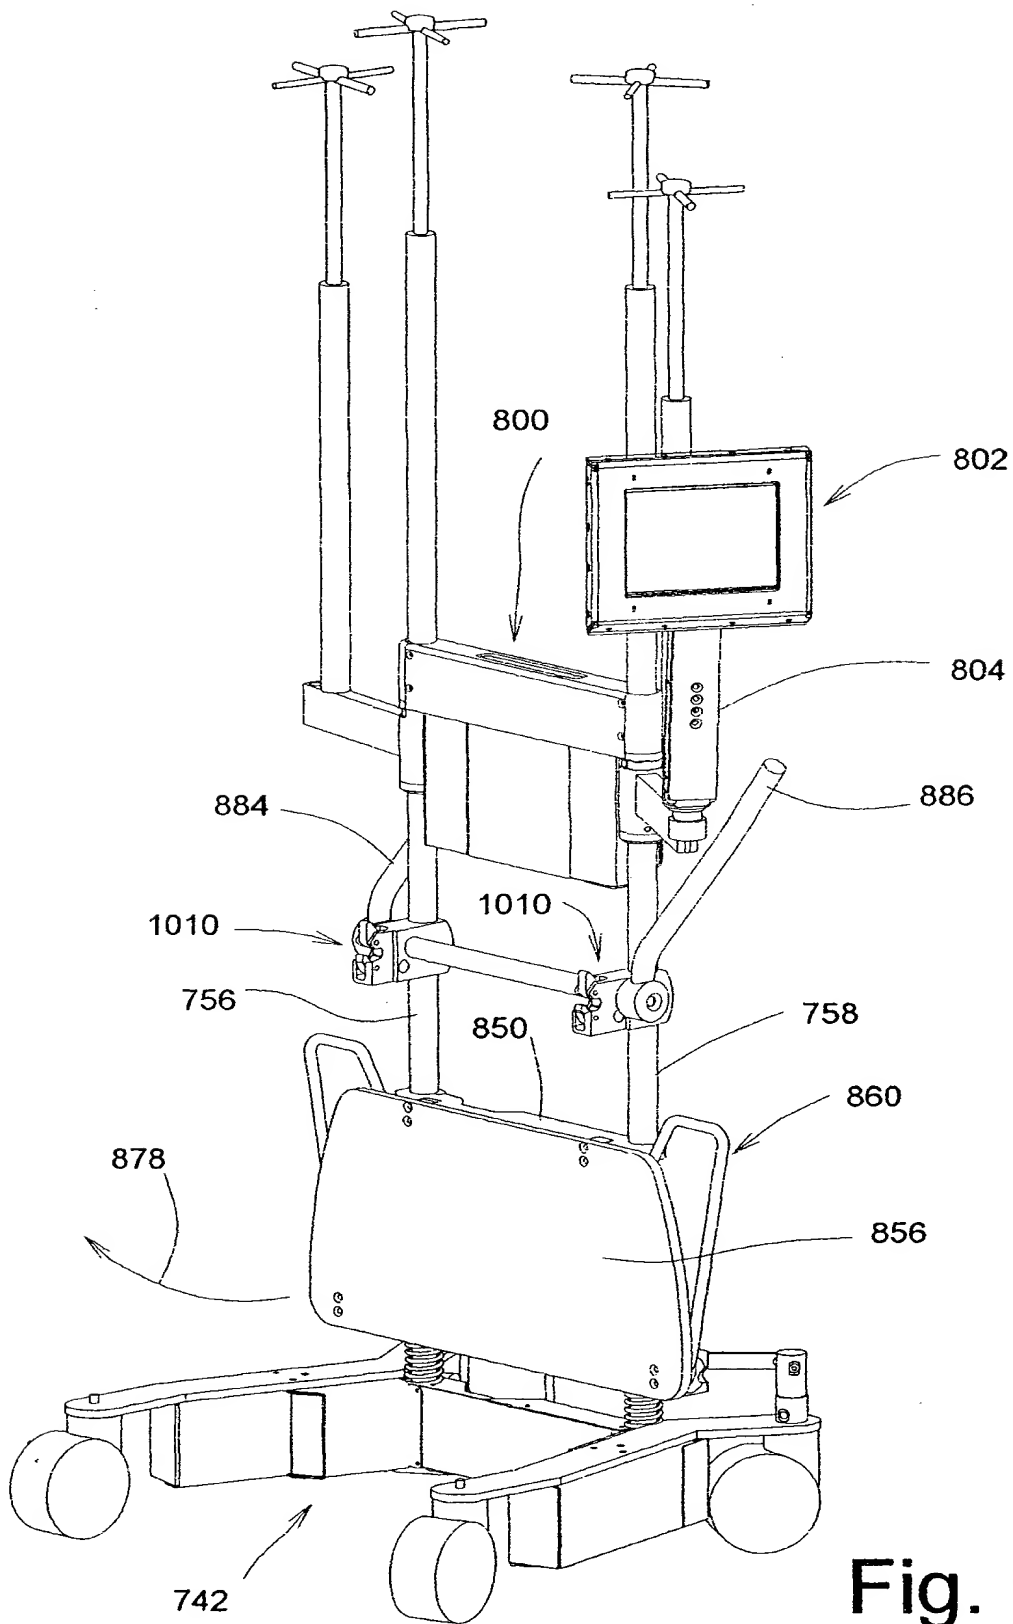


Fig. 54

00849580-121801

39/59

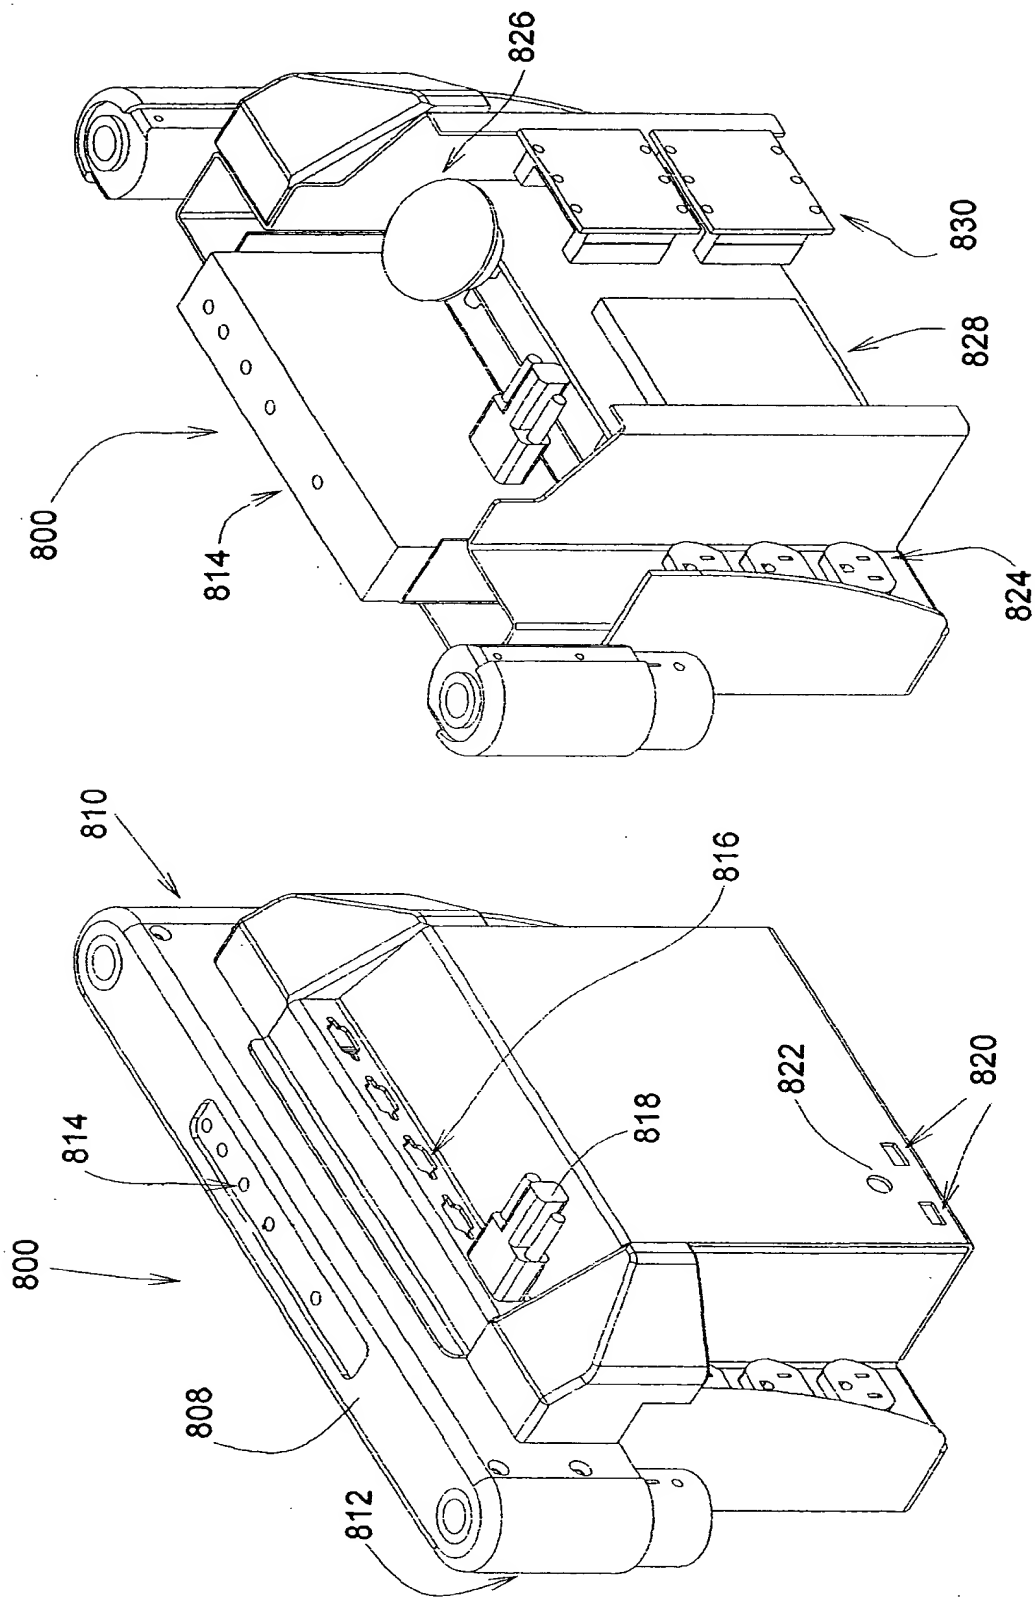


Fig. 56

Fig. 55

40/59

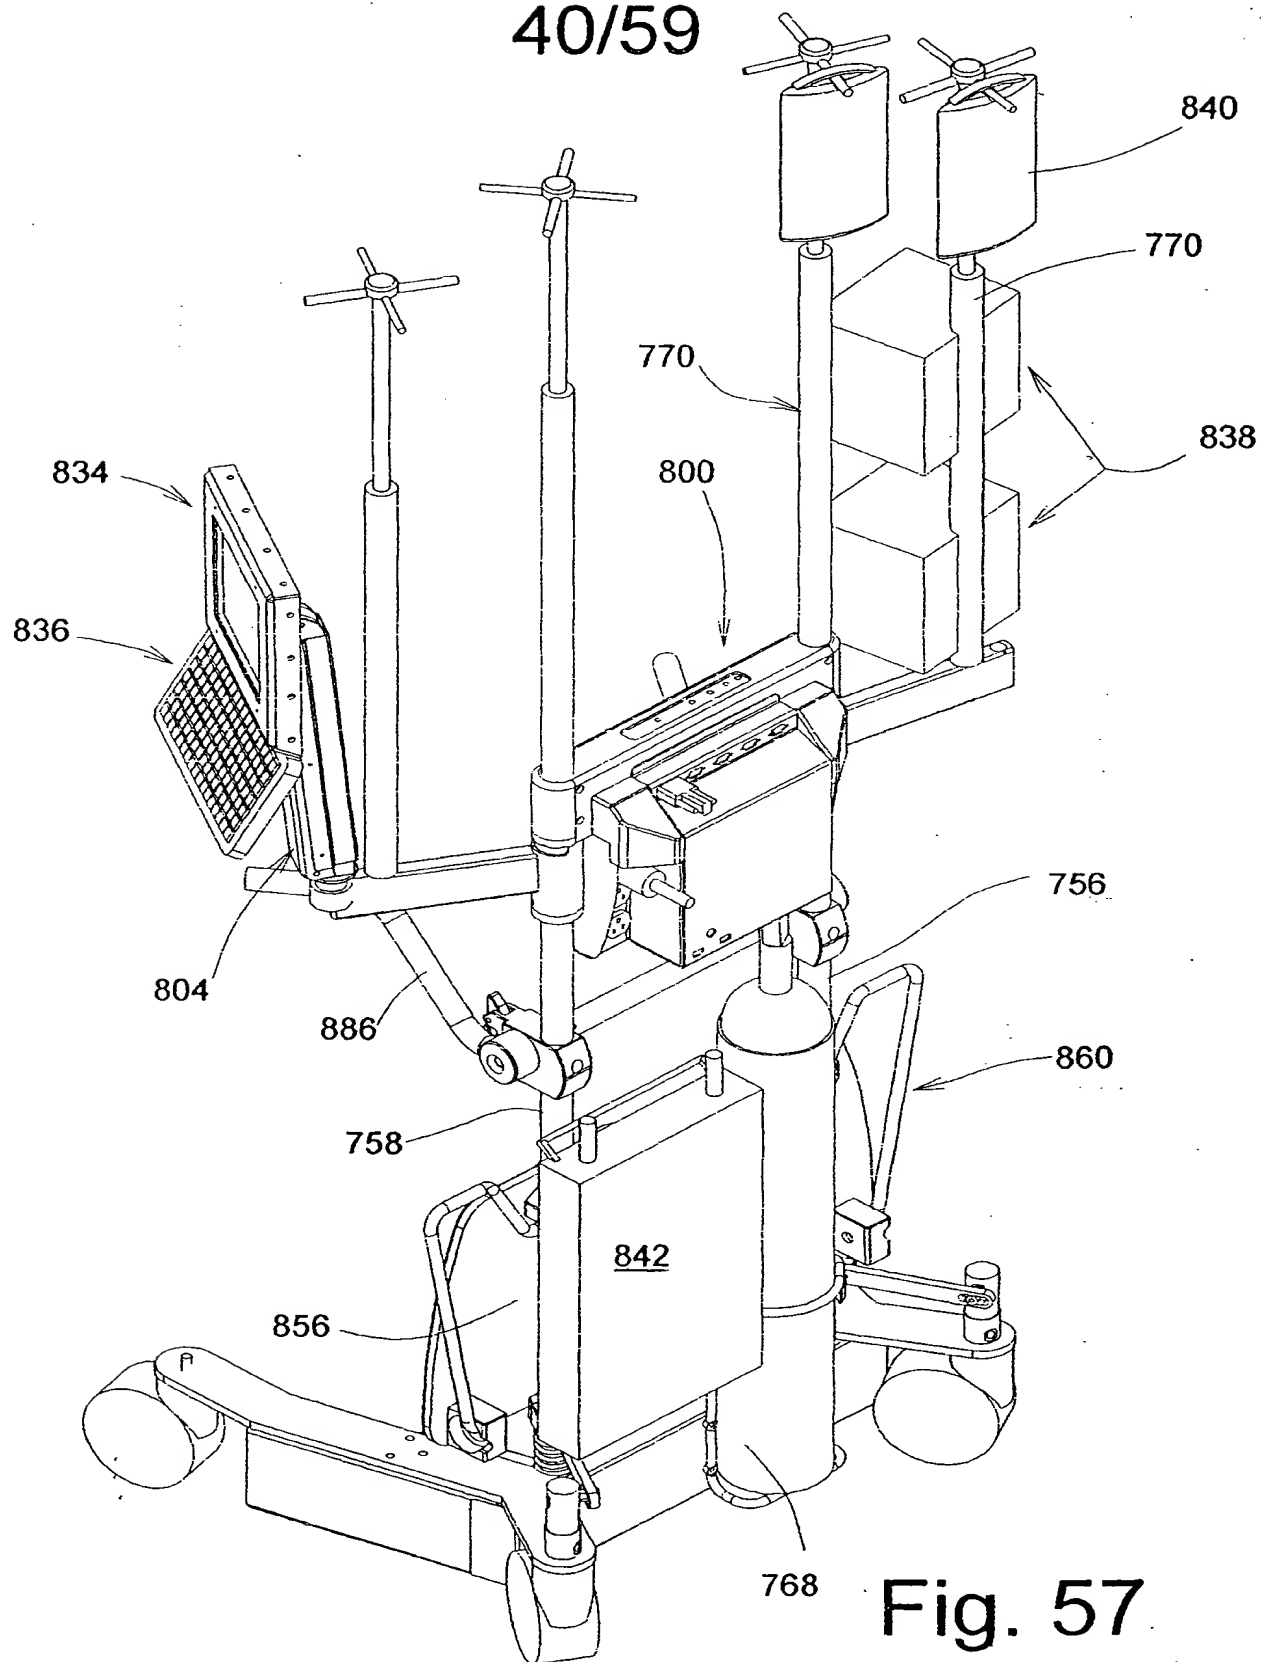


Fig. 57

09849580-121801

41/59


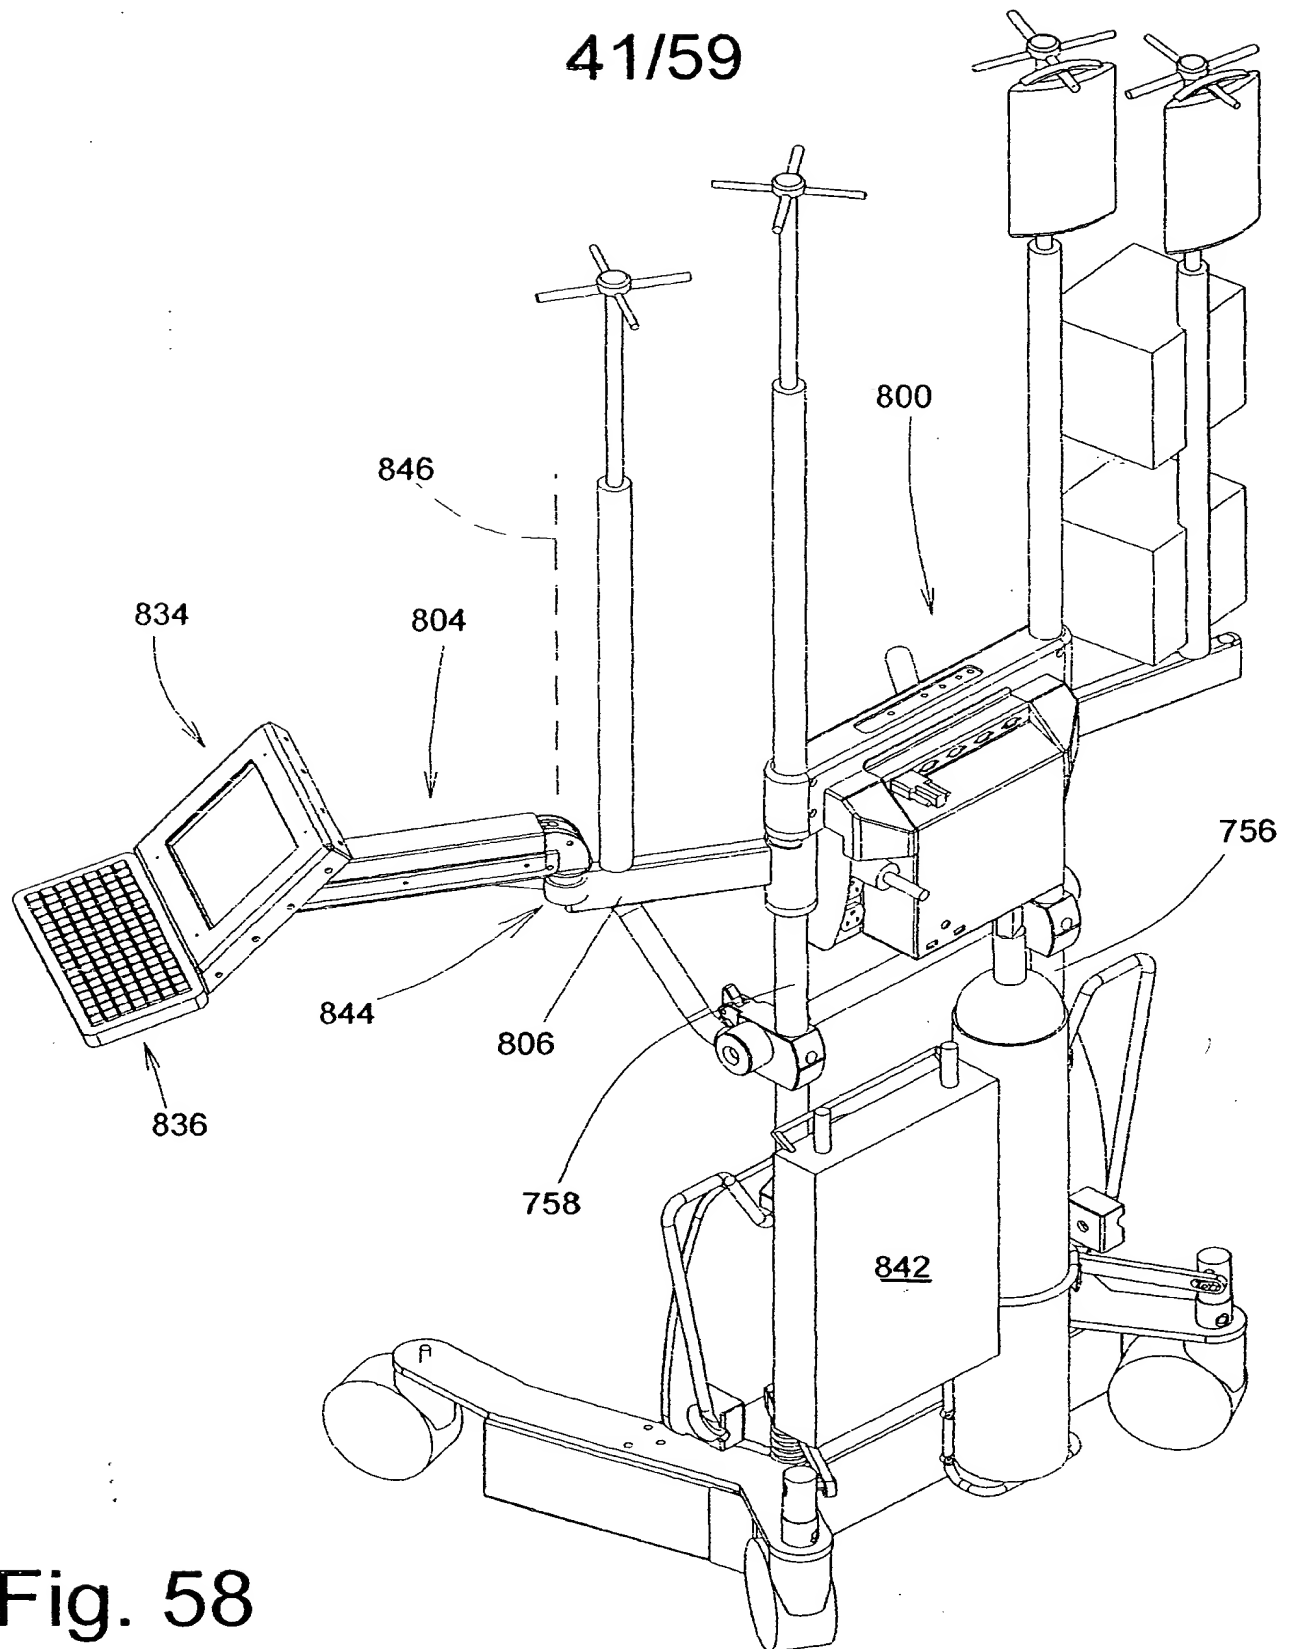


Fig. 58

09849580.121801

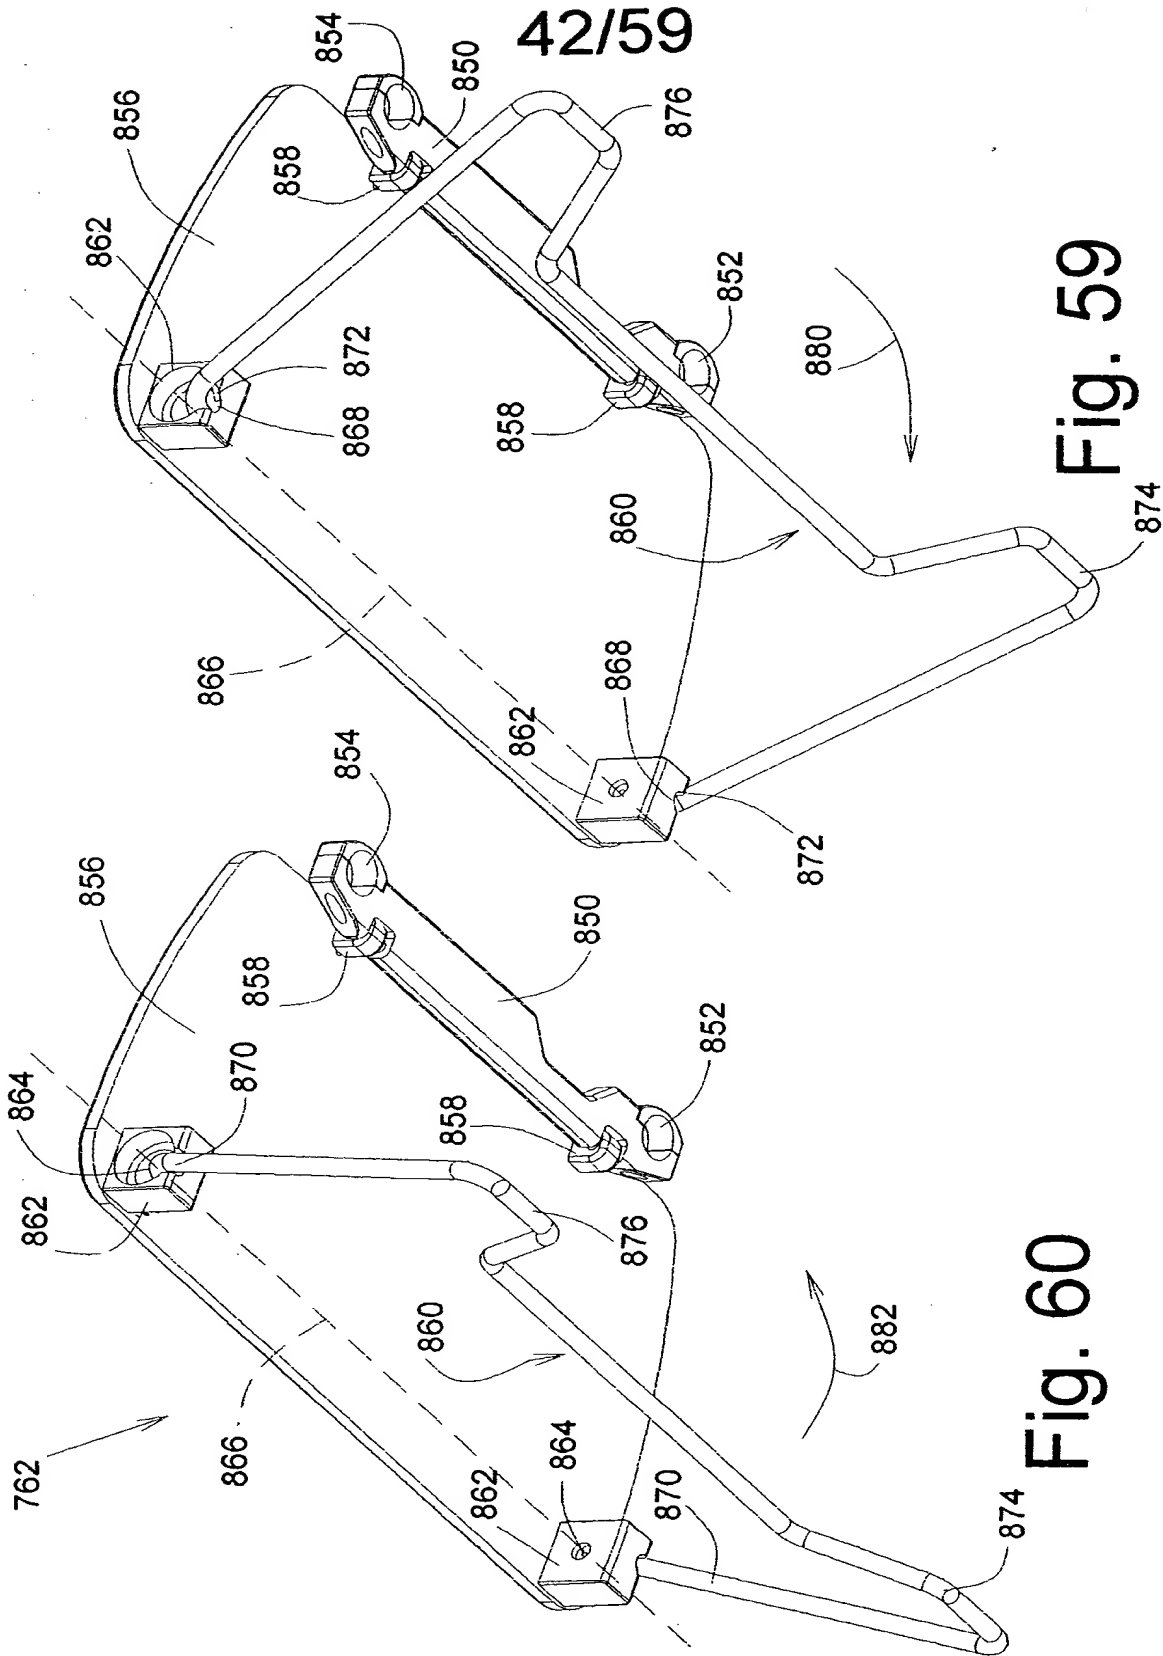

42/59

Fig. 59

Fig. 60

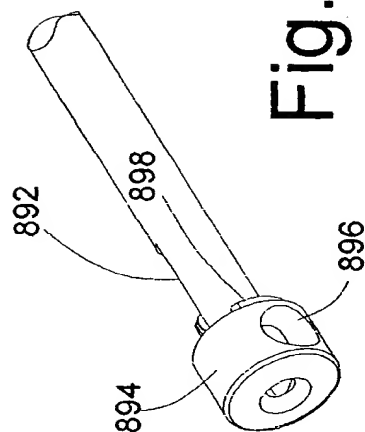
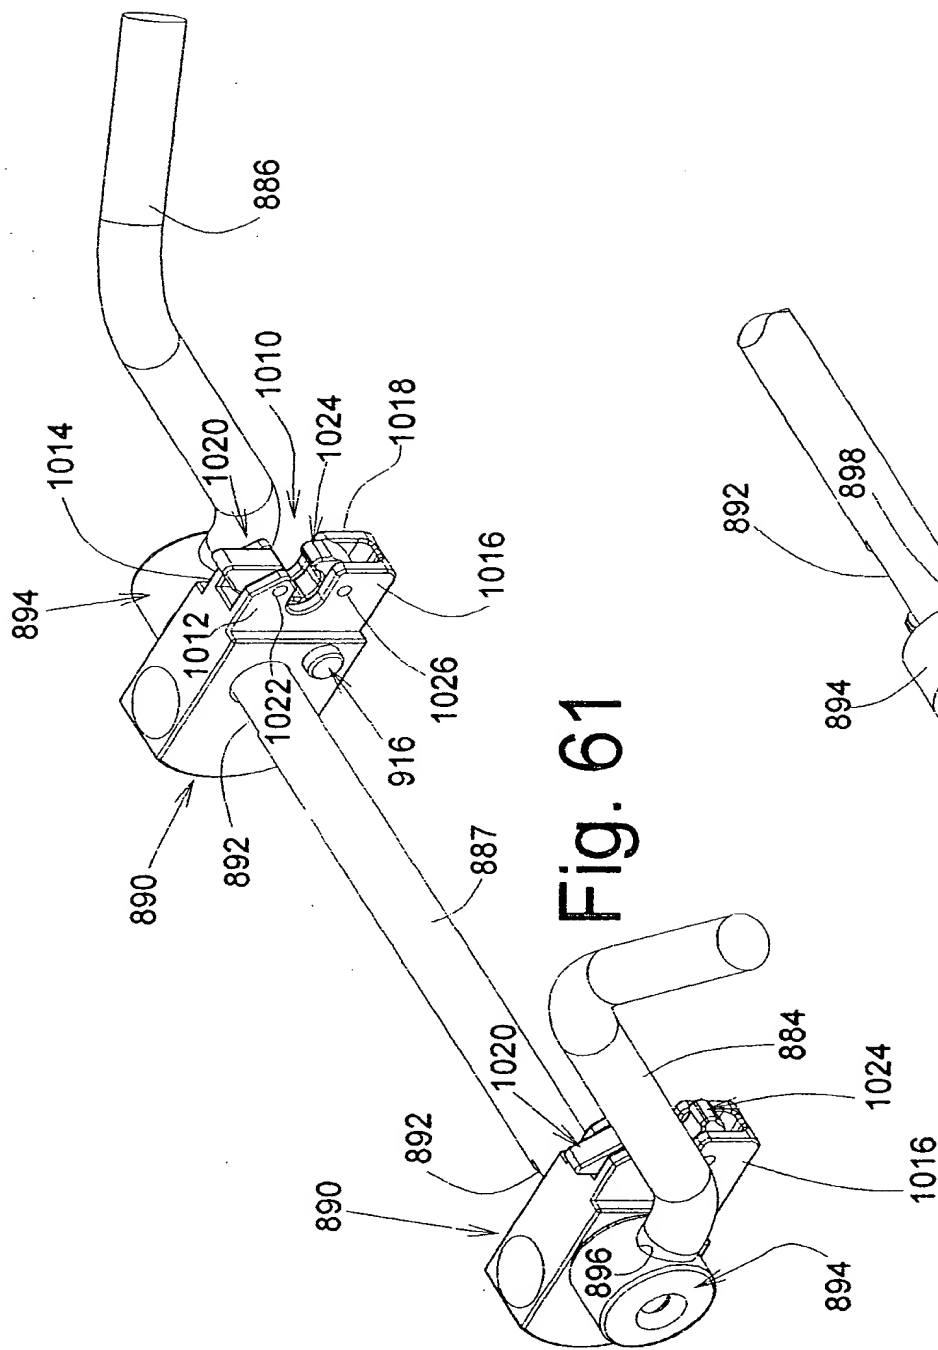


Fig. 63


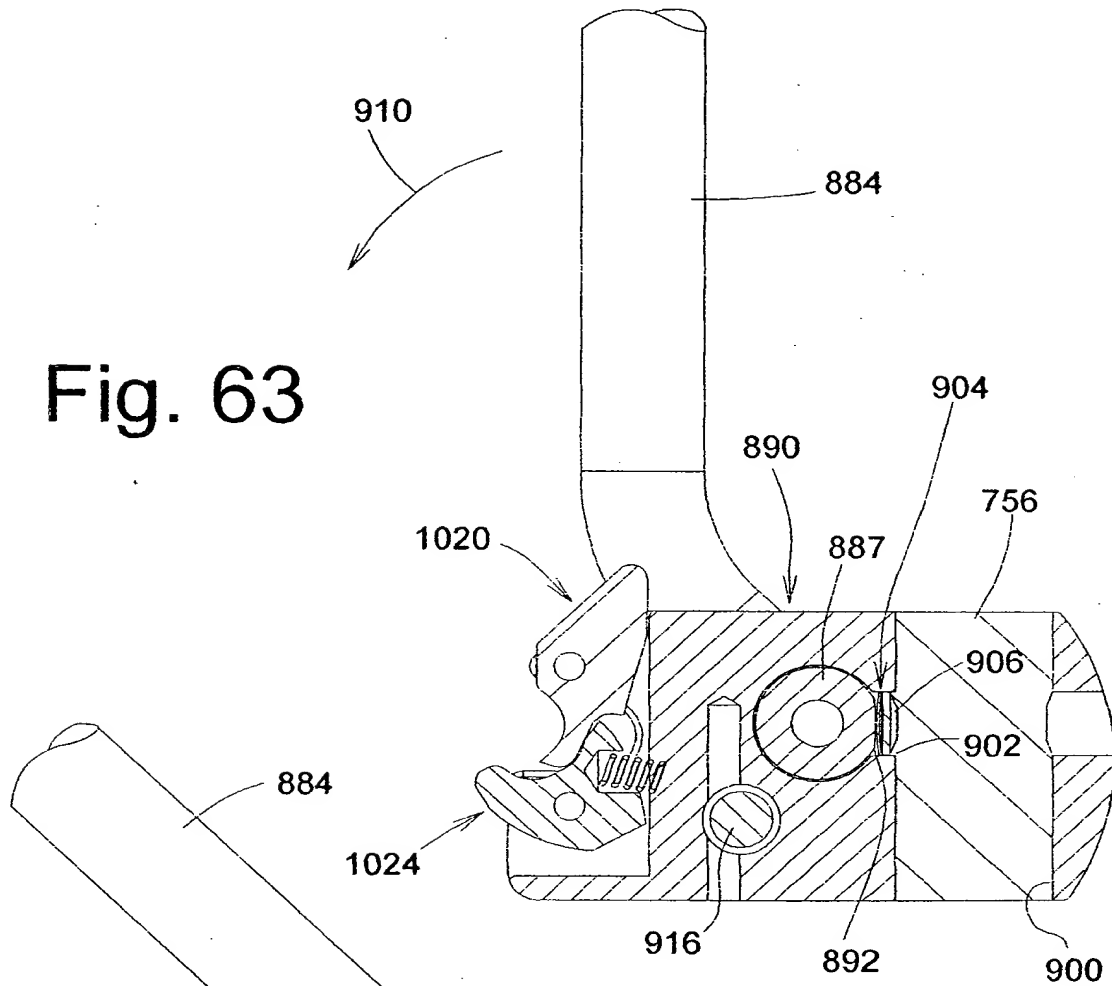


Fig. 64

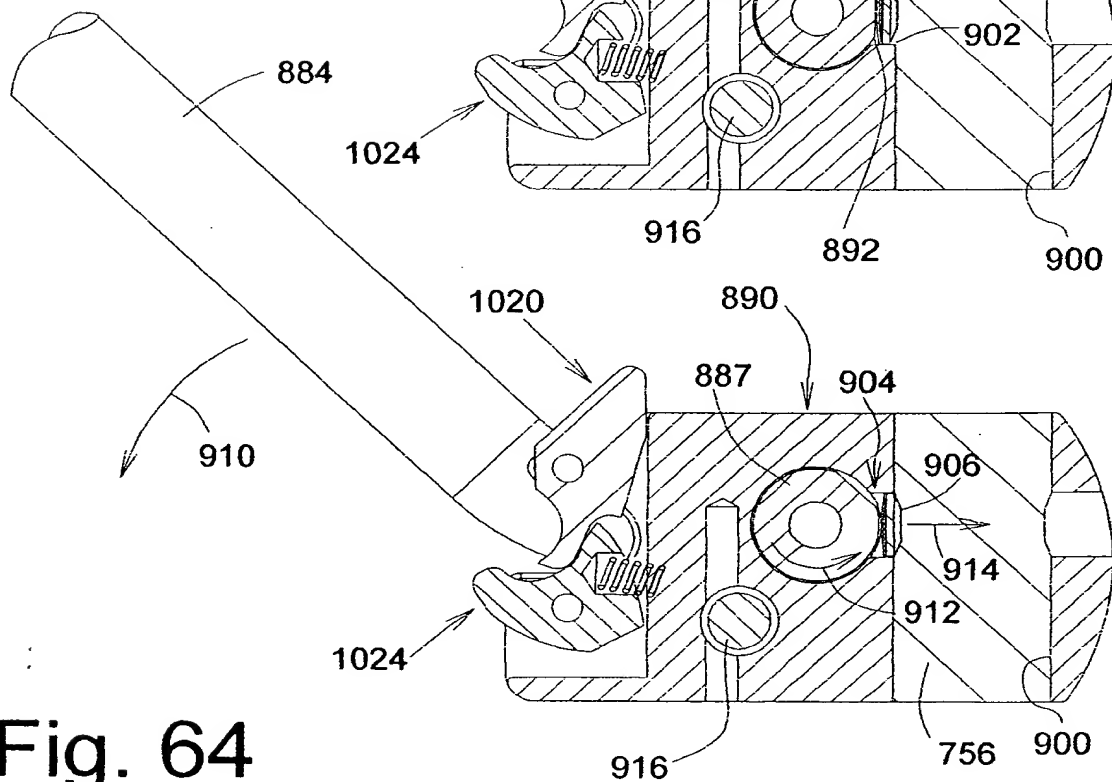

09849580-121801



Fig. 65

46/59

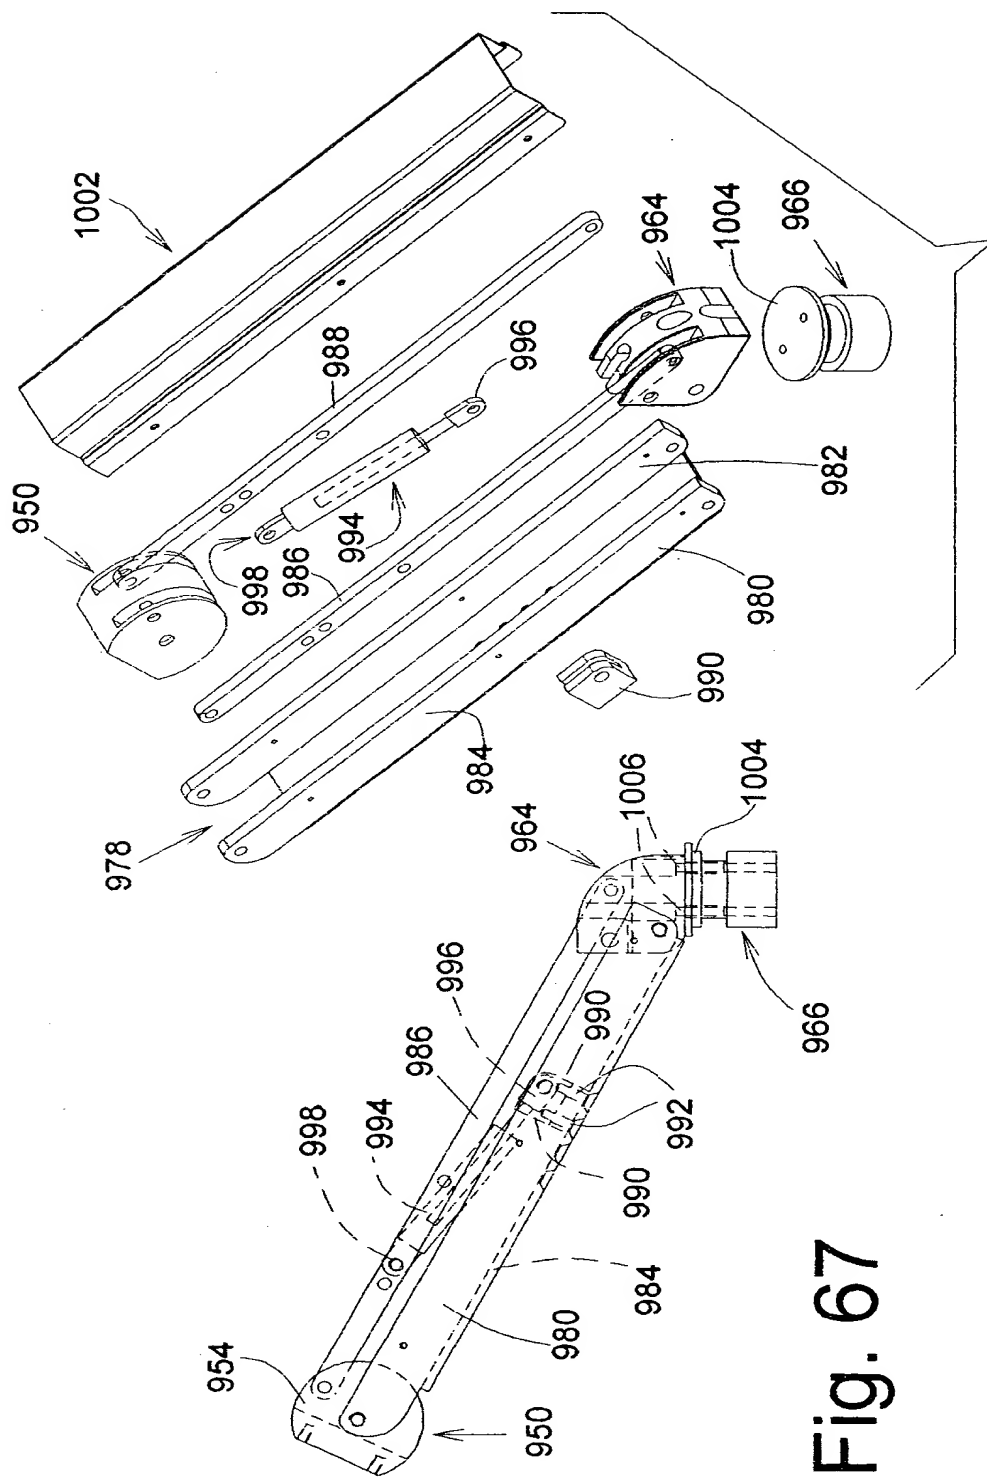


Fig. 67

Fig. 68

47/59

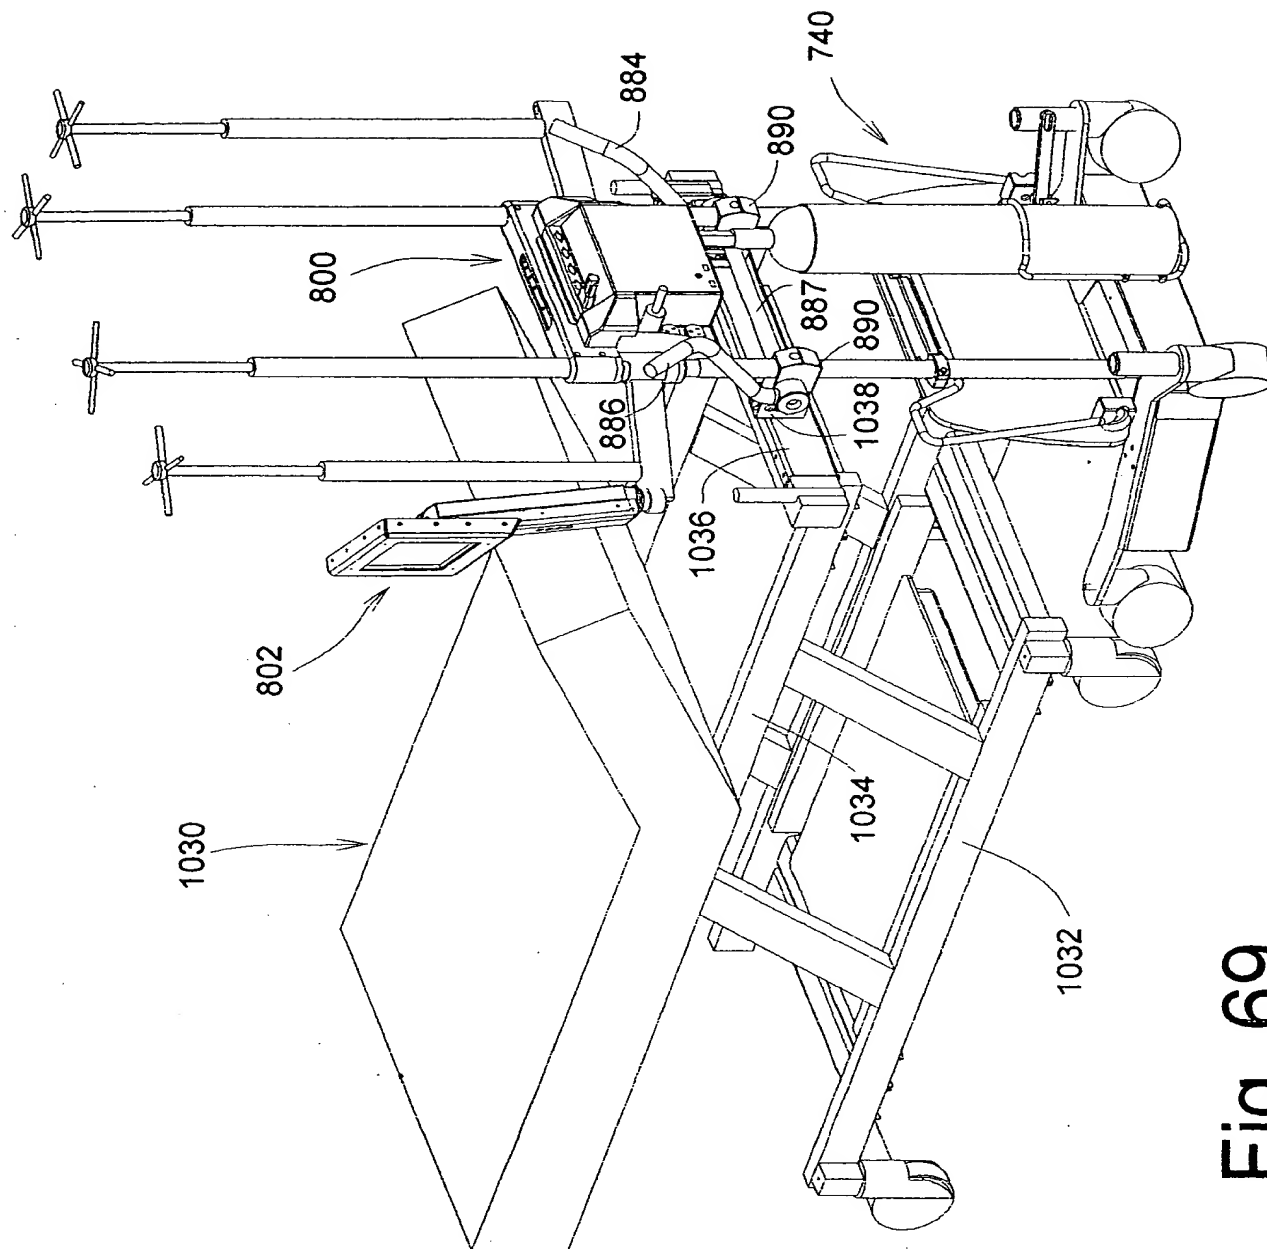


Fig. 69

POSTER 08564860



Fig. 71

Fig. 72

09849580.121801

49/59





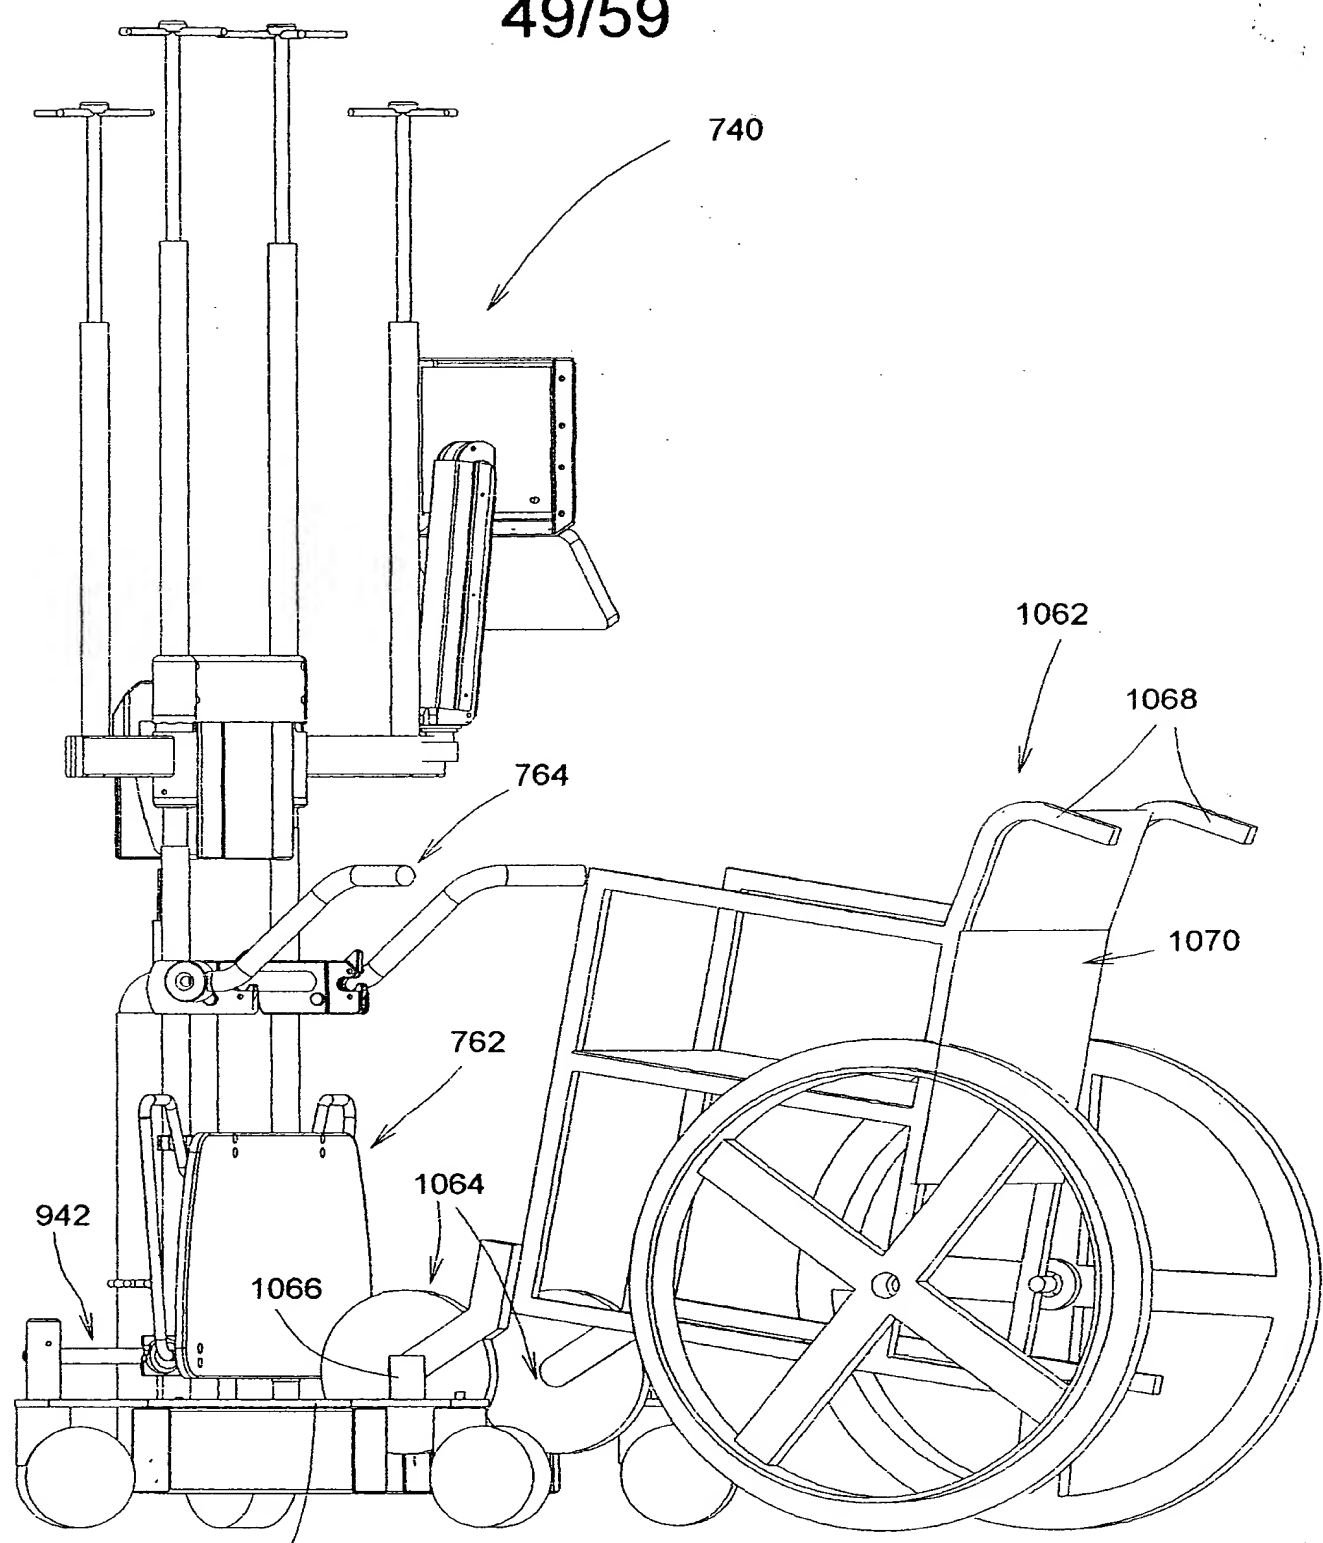


Fig. 73

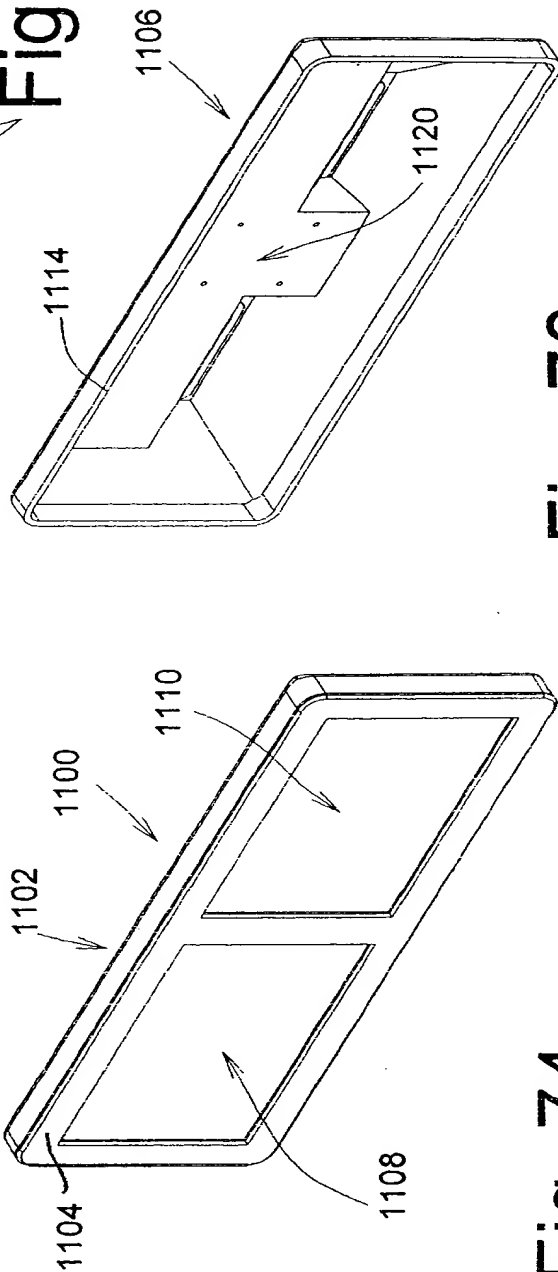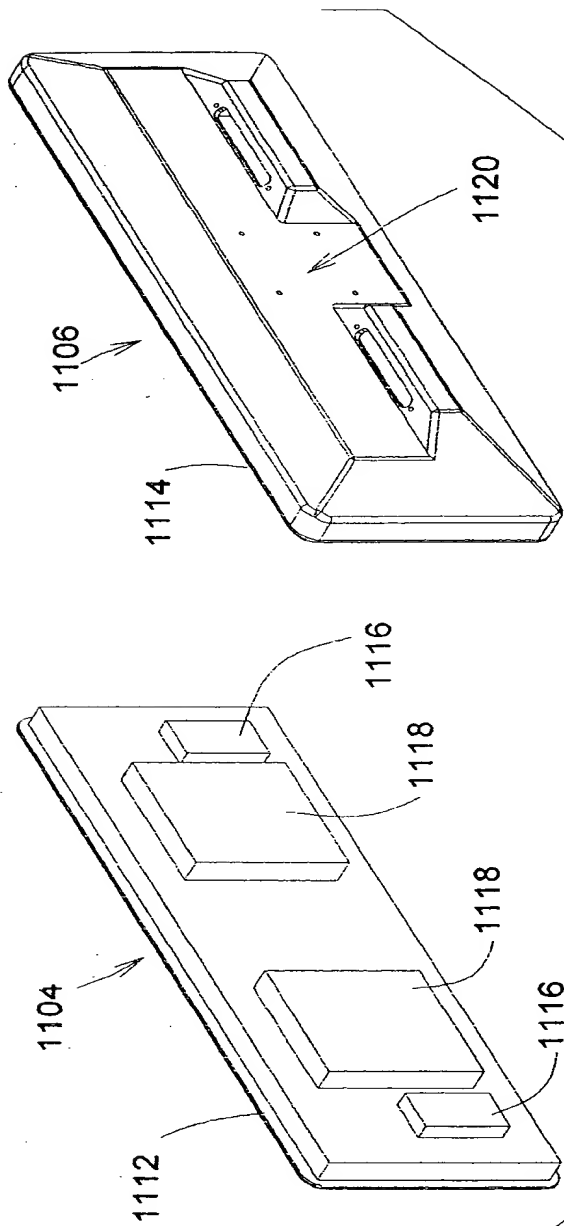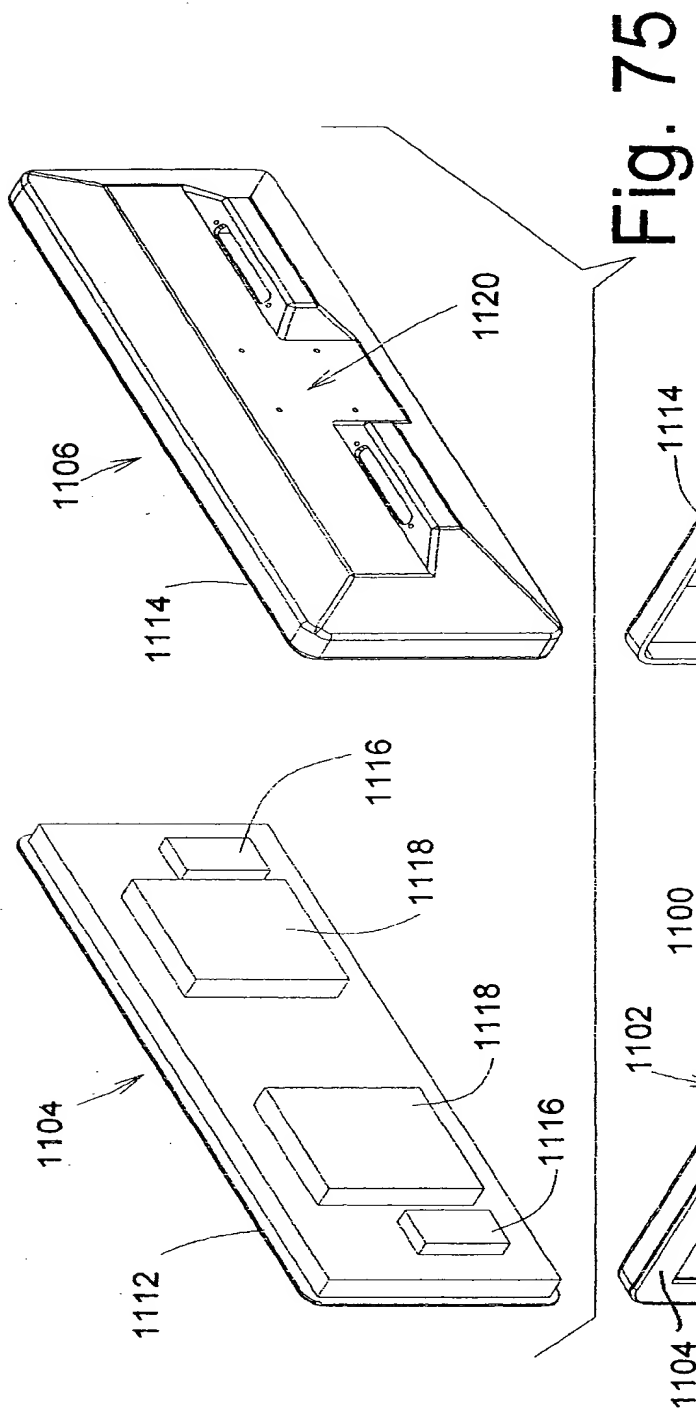

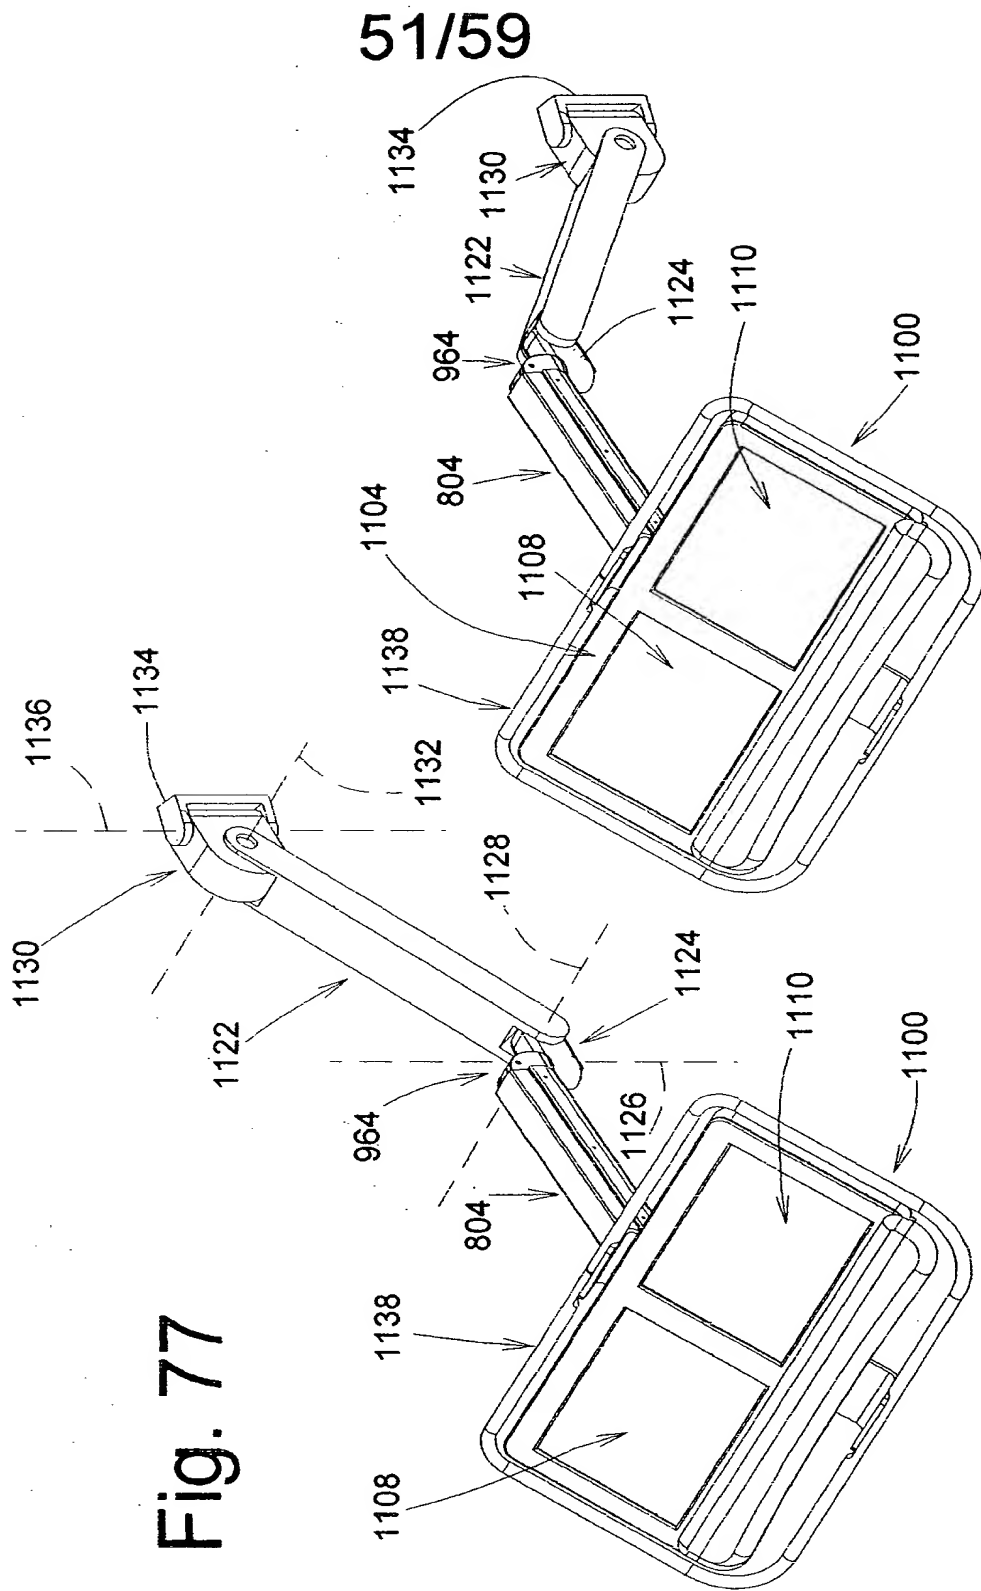

52/59

Fig. 79 A

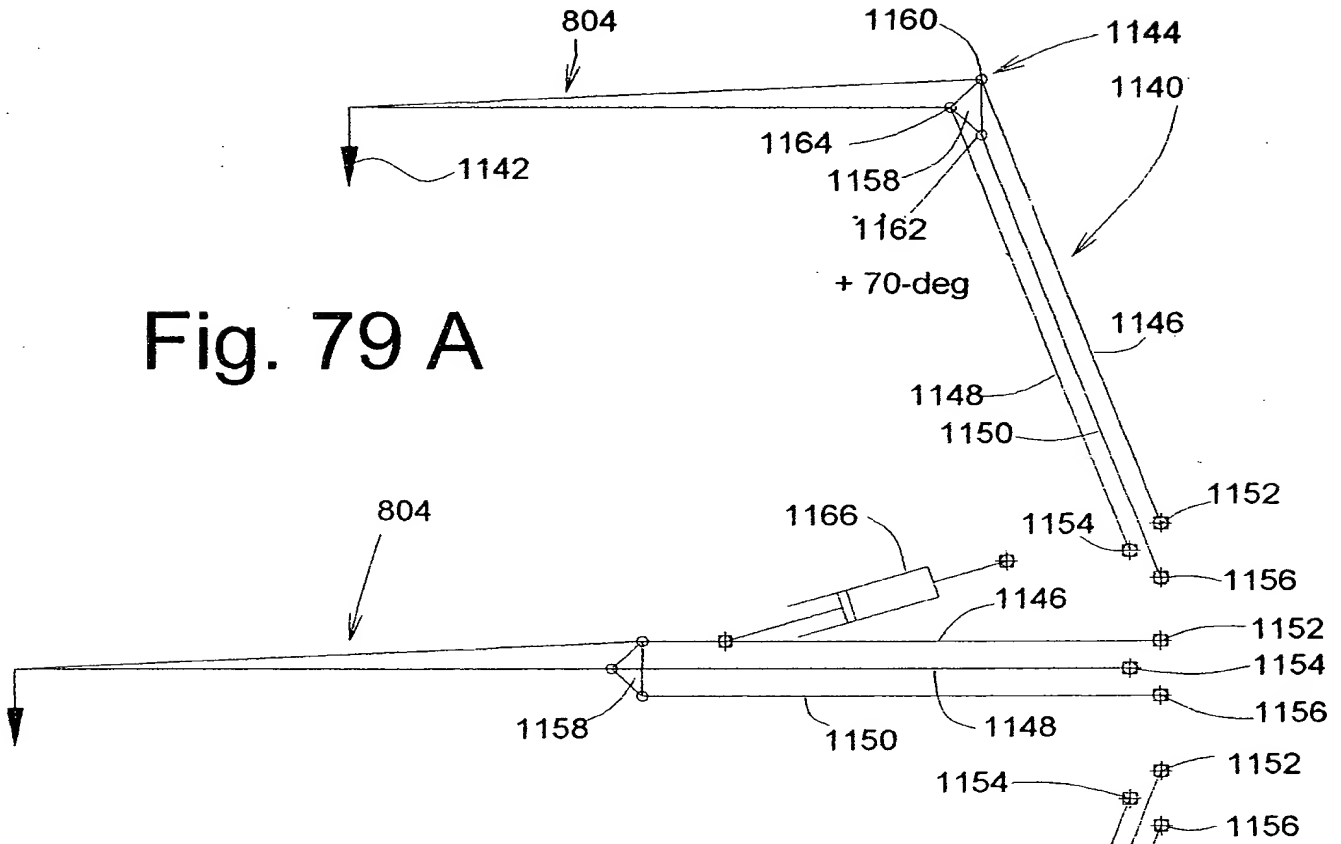


Fig. 79 B

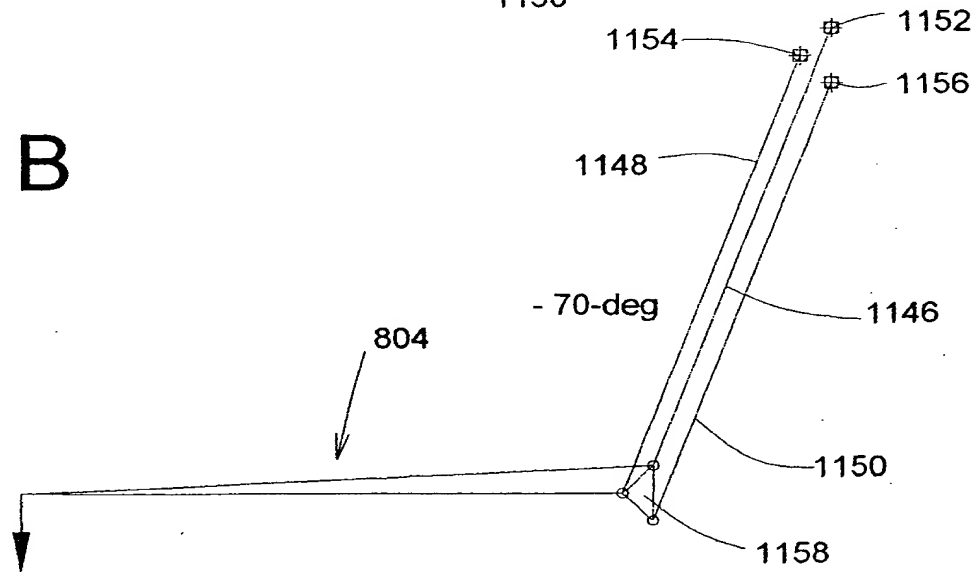


Fig. 79 C

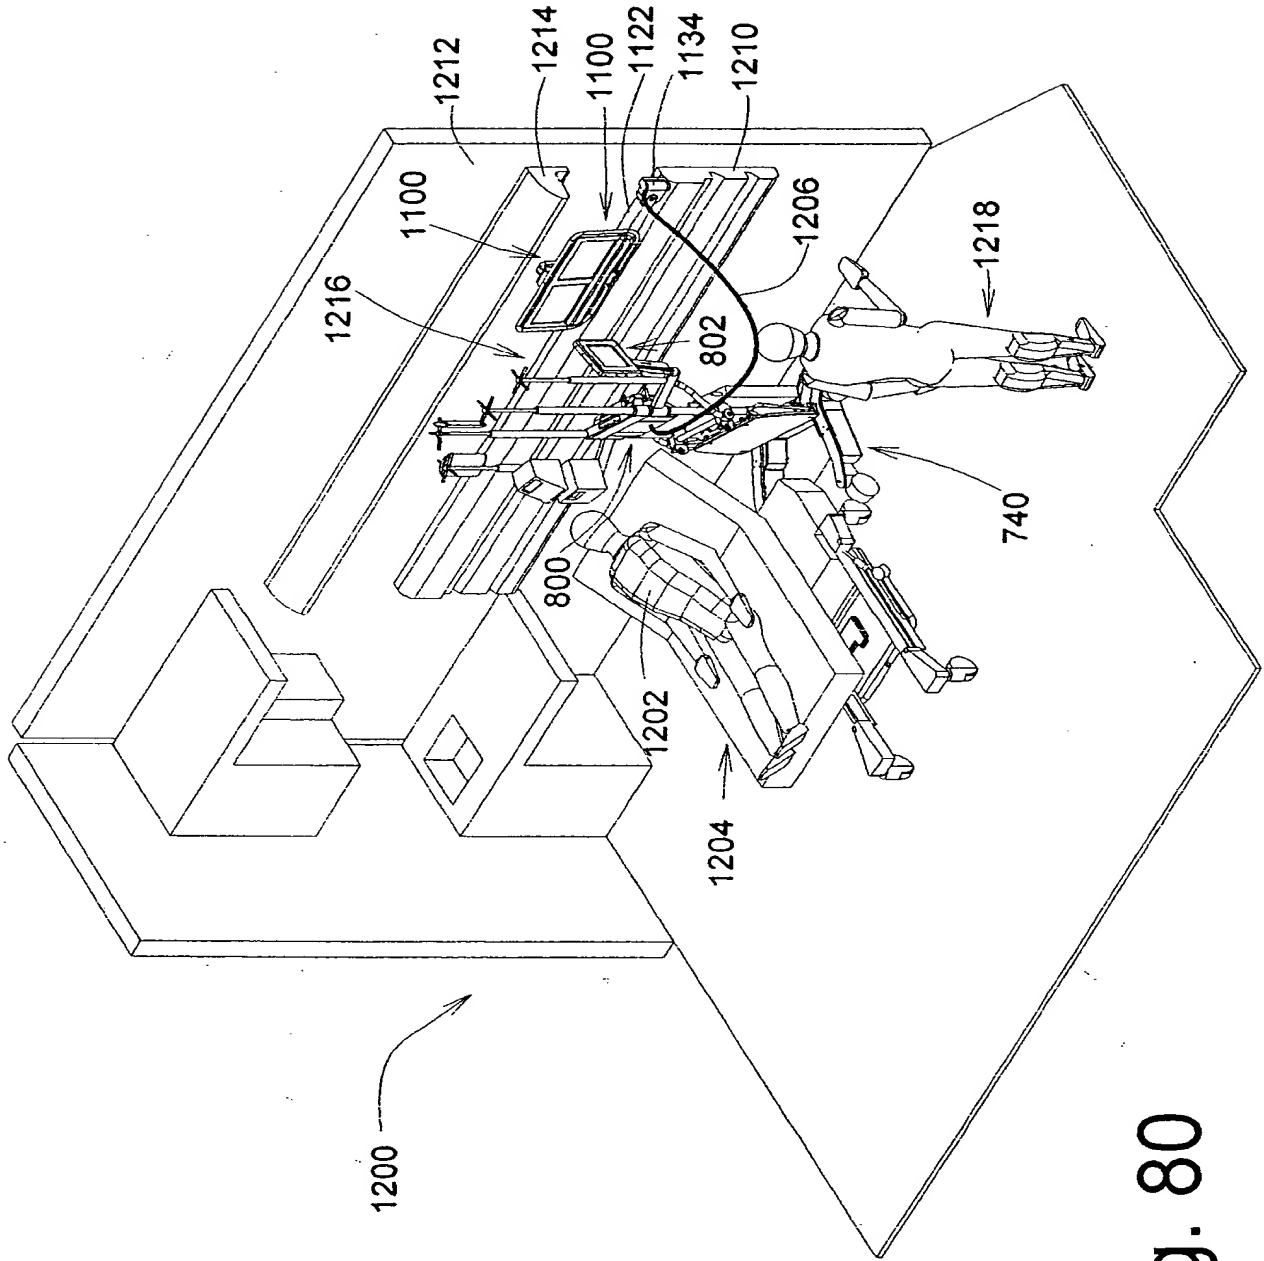


Fig. 80

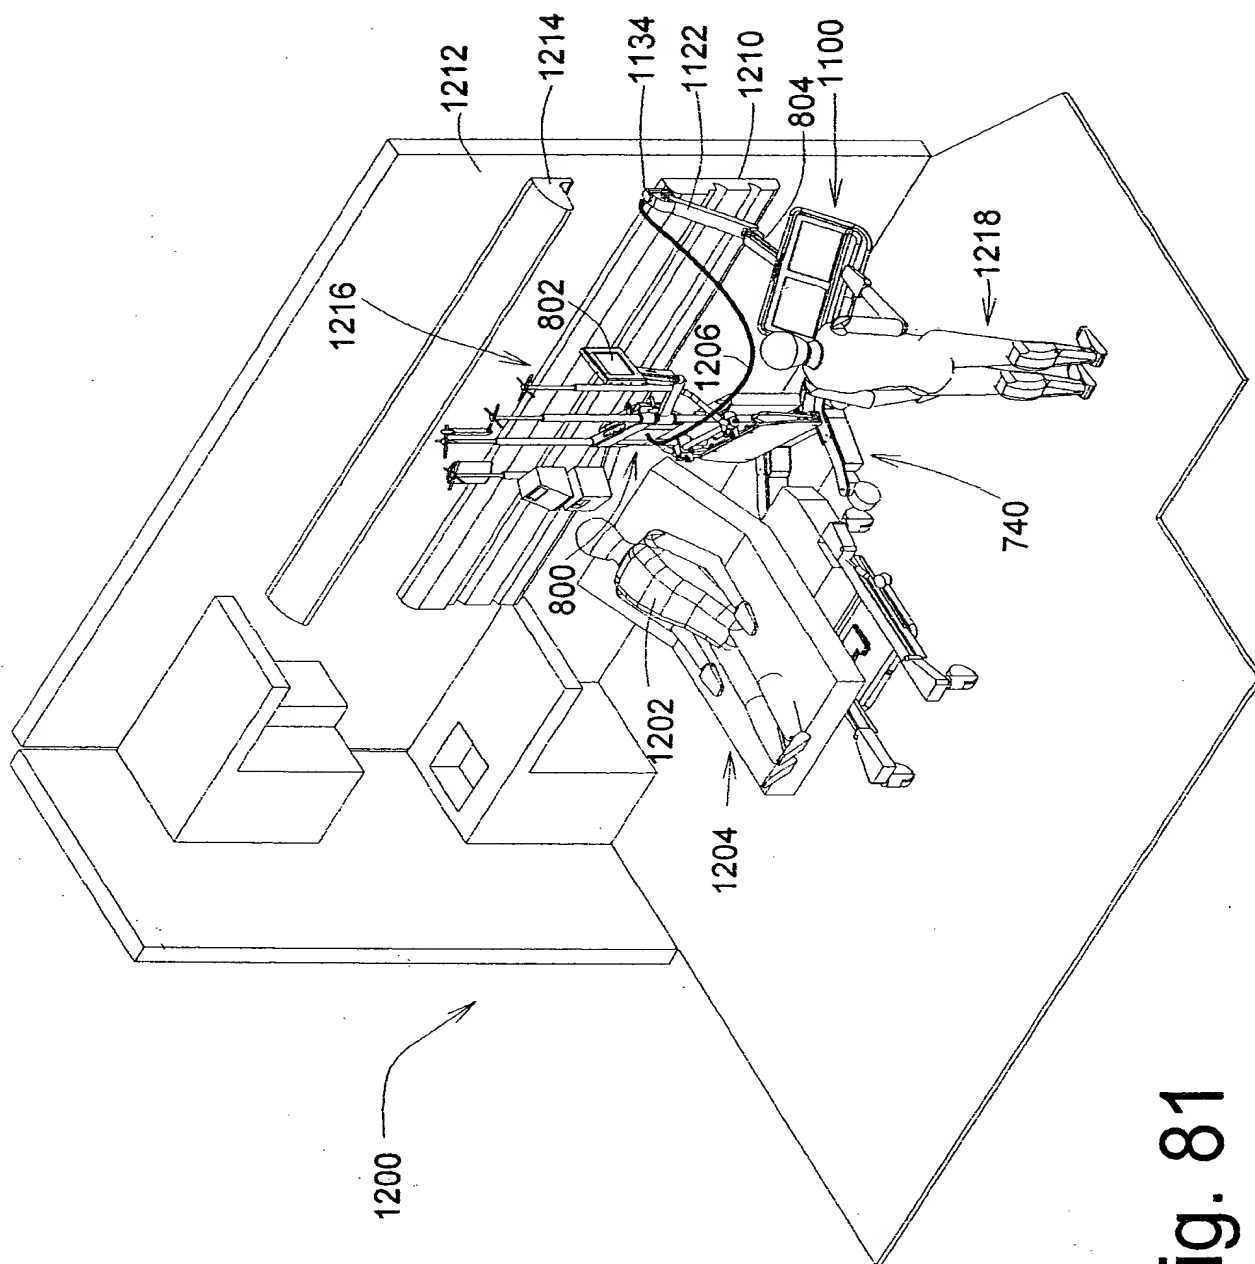


Fig. 81

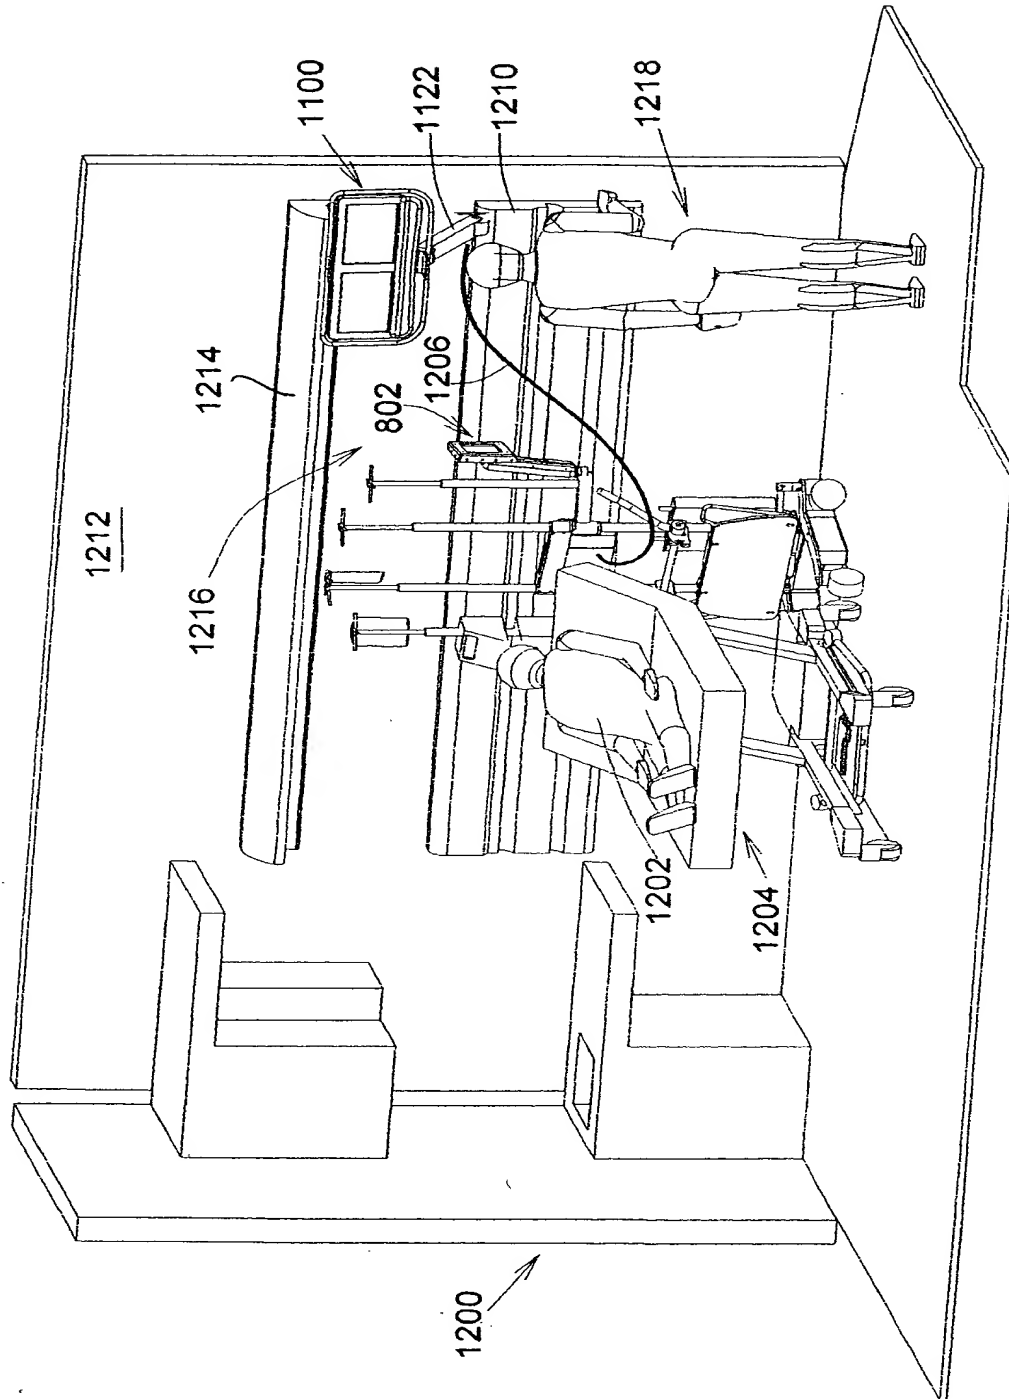


Fig. 82

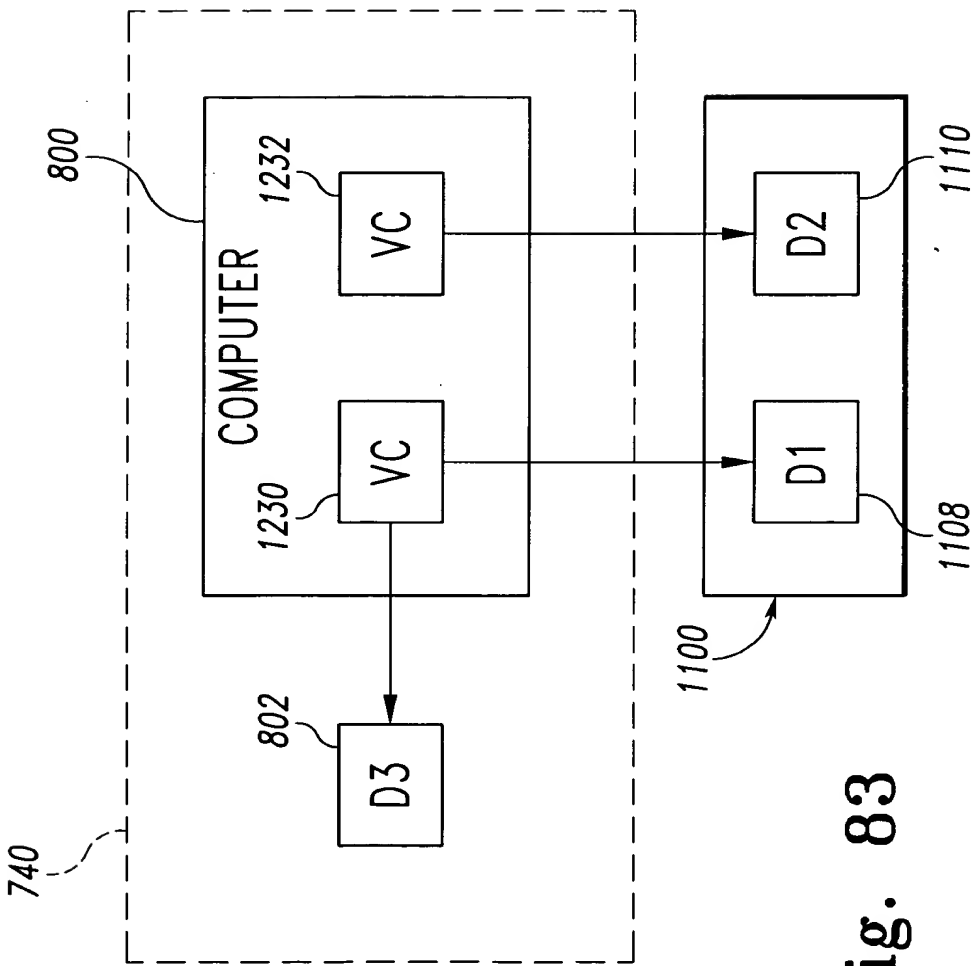


Fig. 83

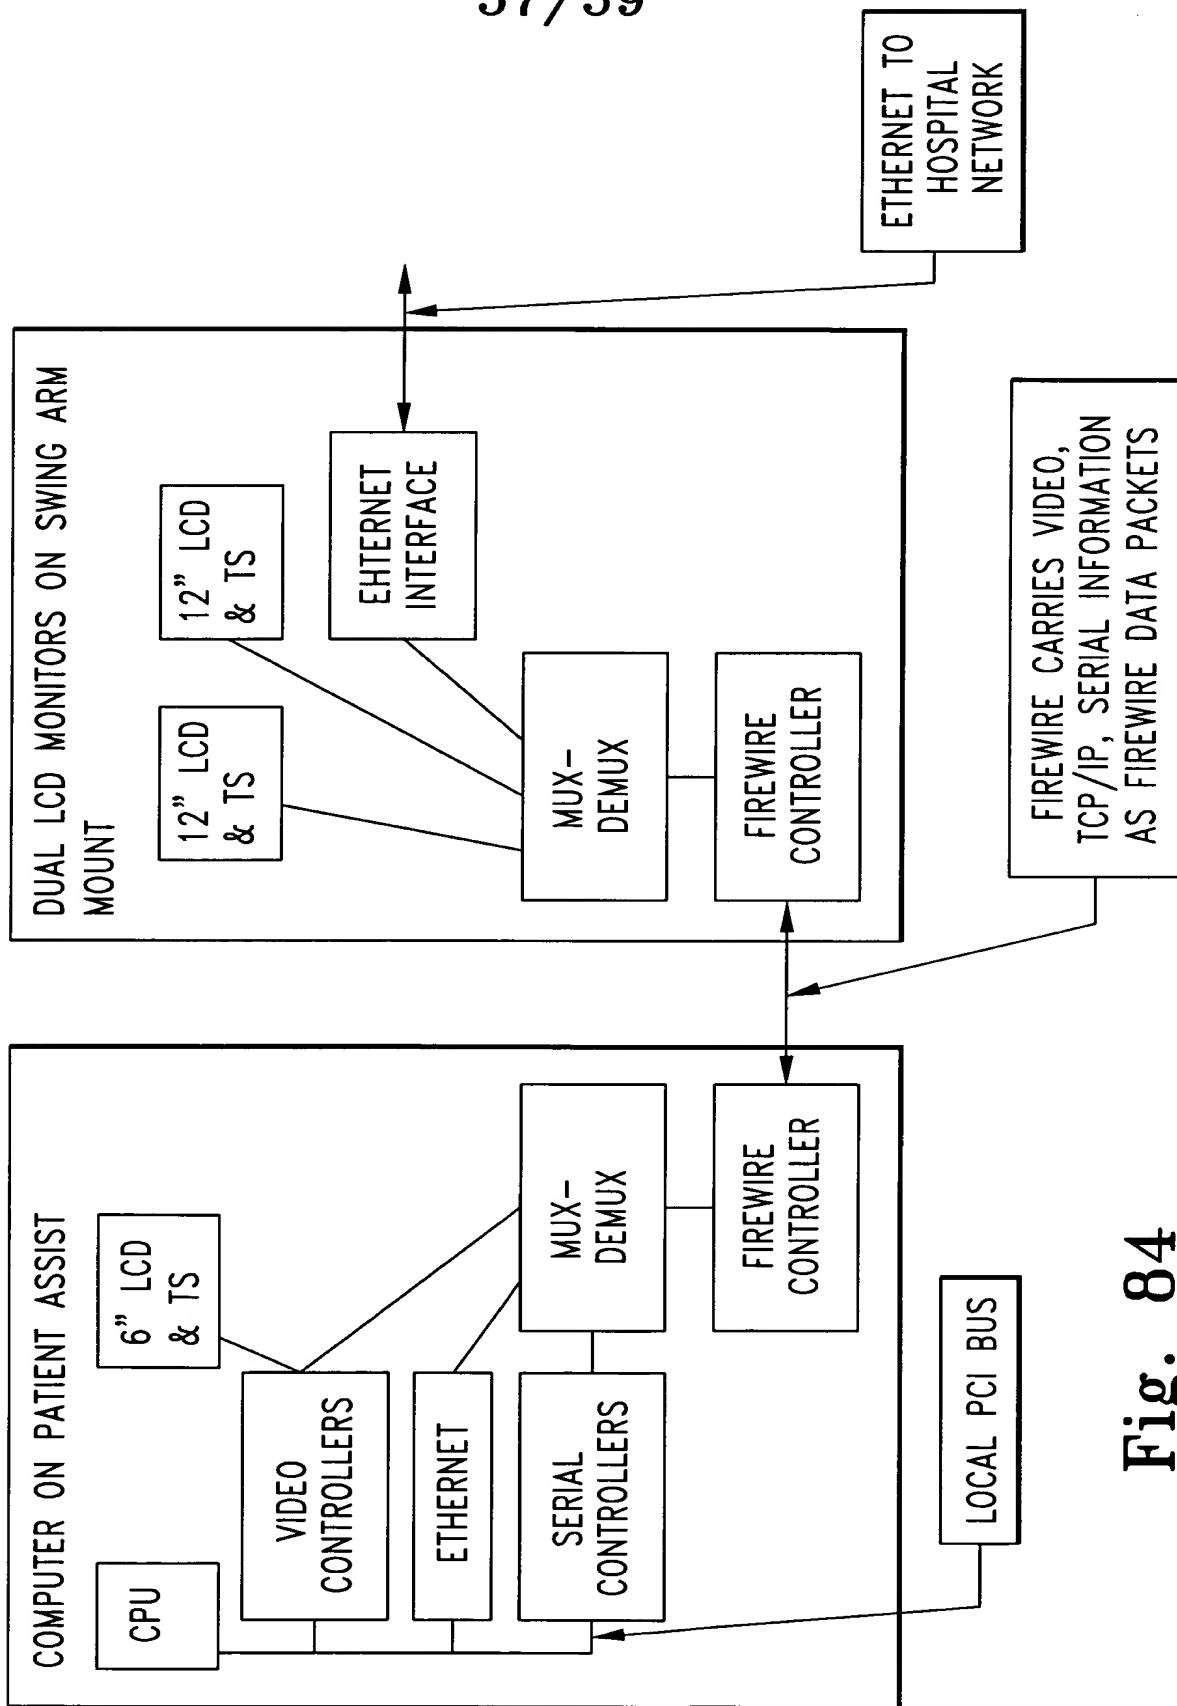


Fig. 84

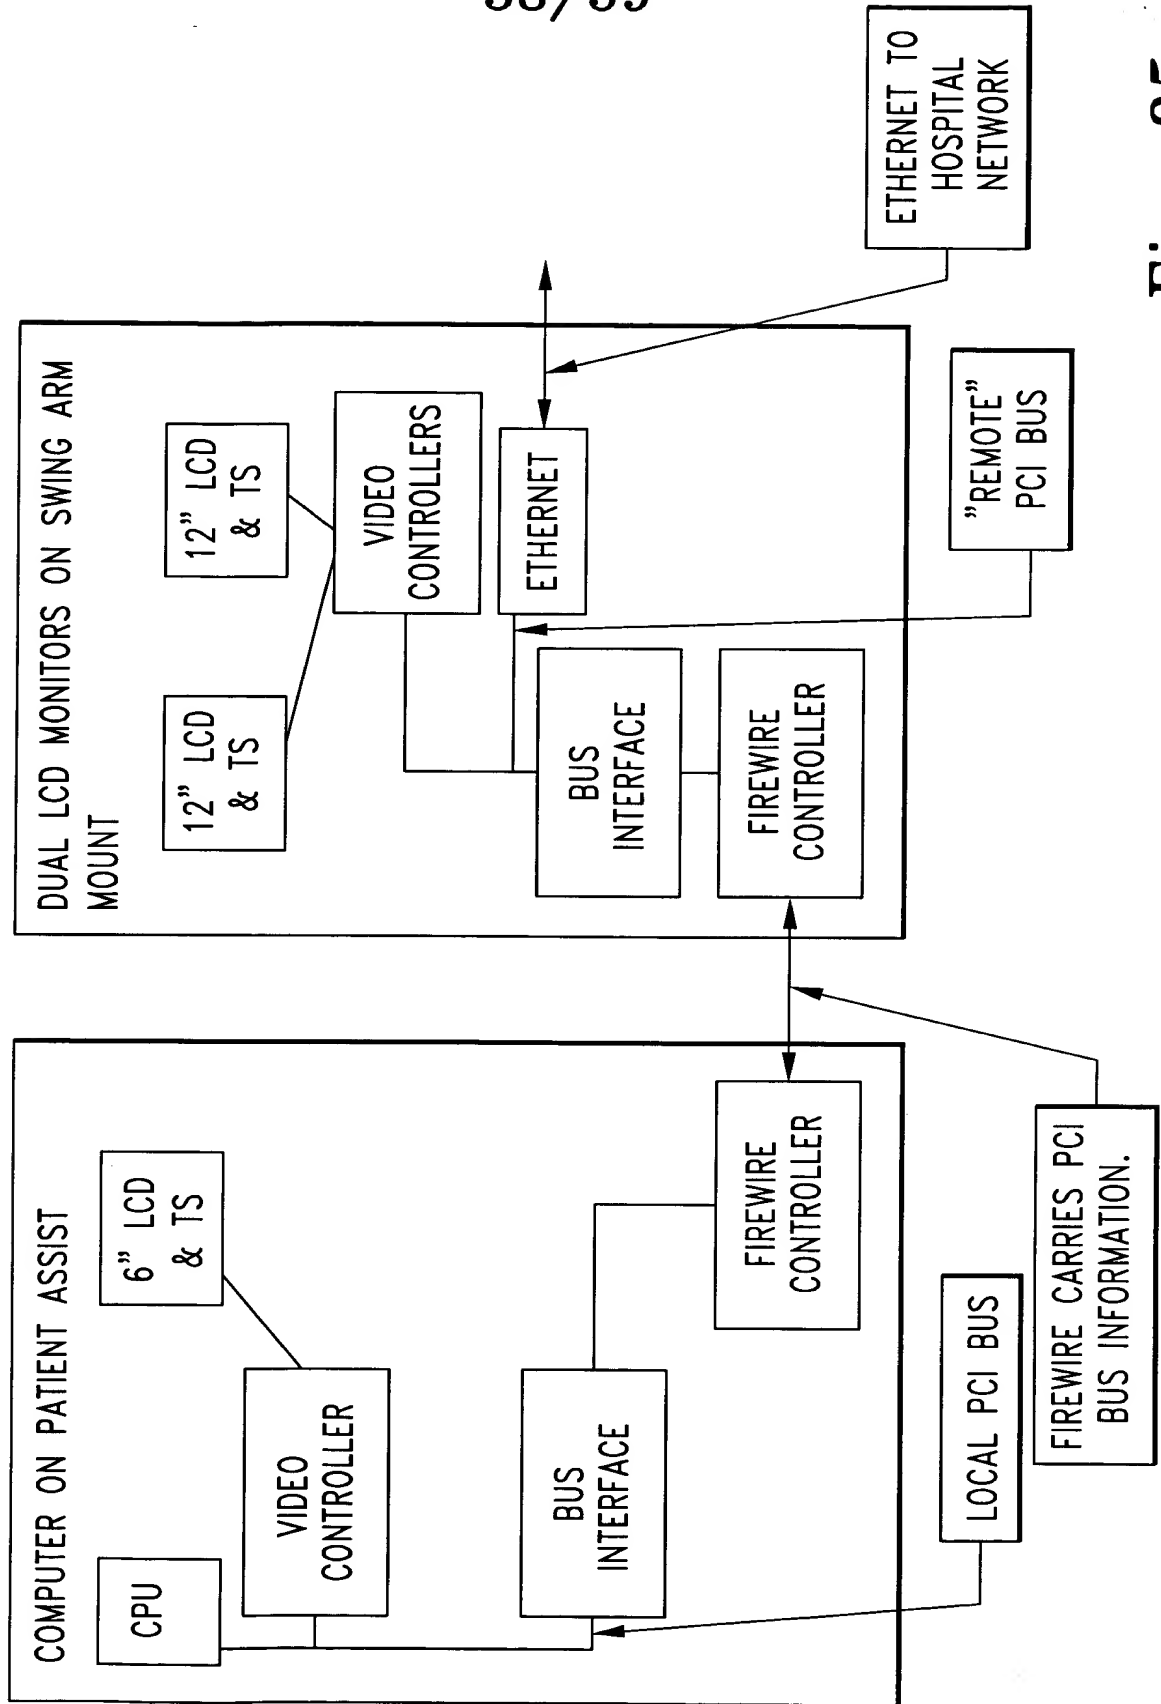


Fig. 85

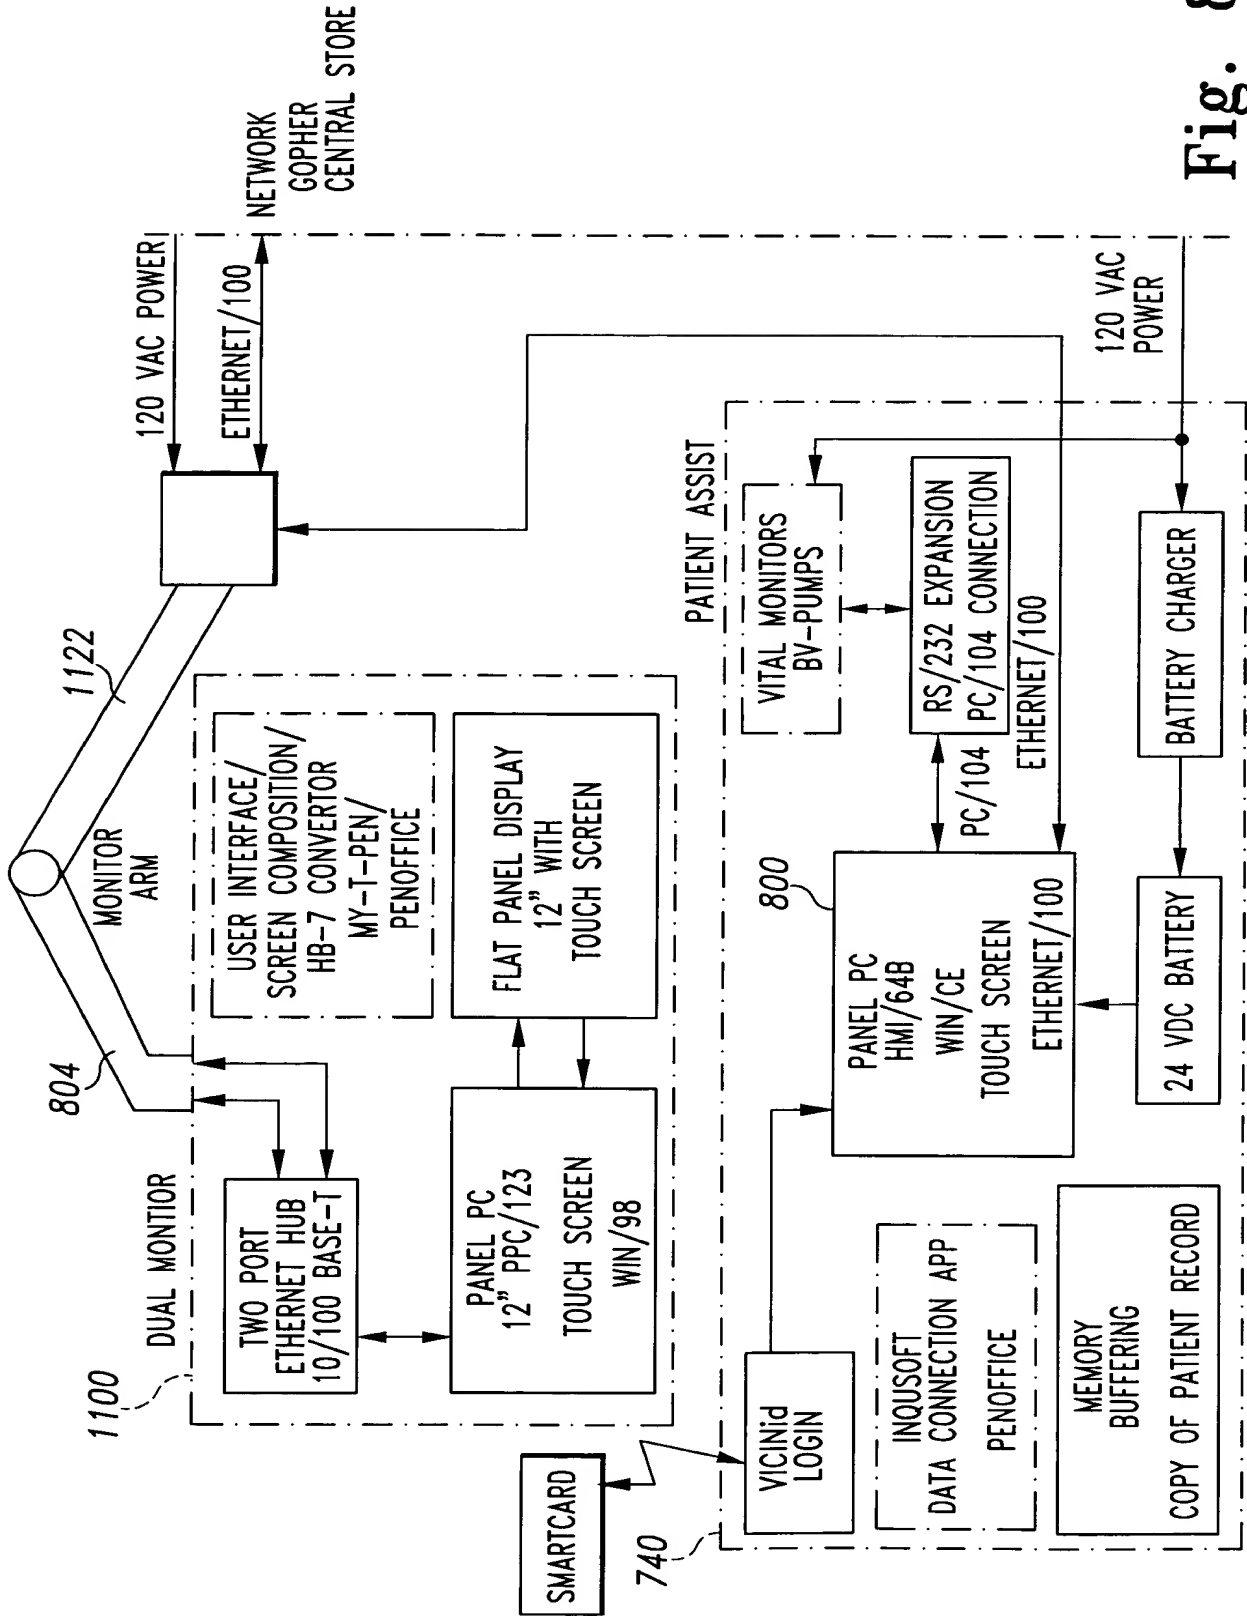


Fig. 86